



Aalborg Universitet

AALBORG UNIVERSITY  
DENMARK

## Electrical energy by electrode placement for cardioversion of atrial fibrillation: a systematic review and meta-analysis

Vinter, Nicklas; Holst-Hansen, Mikkel Zacharias Bystrup; Johnsen, Søren Paaske; Lip, Gregory Y. H.; Frost, Lars; Trinquart, Ludovic

*Published in:*  
Open Heart

*DOI (link to publication from Publisher):*  
[10.1136/openhrt-2023-002456](https://doi.org/10.1136/openhrt-2023-002456)

*Creative Commons License*  
CC BY-NC 4.0

*Publication date:*  
2023

*Document Version*  
Publisher's PDF, also known as Version of record

[Link to publication from Aalborg University](#)

*Citation for published version (APA):*

Vinter, N., Holst-Hansen, M. Z. B., Johnsen, S. P., Lip, G. Y. H., Frost, L., & Trinquart, L. (2023). Electrical energy by electrode placement for cardioversion of atrial fibrillation: a systematic review and meta-analysis. *Open Heart*, 10(2), Article e002456. <https://doi.org/10.1136/openhrt-2023-002456>

### General rights





Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal -

### Take down policy

If you believe that this document breaches copyright please contact us at [vbn@aub.aau.dk](mailto:vbn@aub.aau.dk) providing details, and we will remove access to the work immediately and investigate your claim.

# openheart Electrical energy by electrode placement for cardioversion of atrial fibrillation: a systematic review and meta-analysis

Nicklas Vinter <sup>1,2,3</sup>, Mikkel Zacharias Bystrup Holst-Hansen,<sup>1</sup>  
Søren Paaske Johnsen <sup>3</sup>, Gregory Y H Lip <sup>3,4</sup>, Lars Frost <sup>1,2</sup>,  
Ludovic Trinquart <sup>3,5,6</sup>

► Additional supplemental material is published online only. To view, please visit the journal online (<http://dx.doi.org/10.1136/openhrt-2023-002456>).

**To cite:** Vinter N, Holst-Hansen MZB, Johnsen SP, *et al.* Electrical energy by electrode placement for cardioversion of atrial fibrillation: a systematic review and meta-analysis. *Open Heart* 2023;**10**:e002456. doi:10.1136/openhrt-2023-002456

Received 11 August 2023  
Accepted 26 October 2023

## ABSTRACT

**Objective** Electrode patch position may not be critical for success when cardioverting atrial fibrillation (AF), but the relevance of applied electrical energy is unclarified. Our objective was to perform a meta-analysis of randomised trials to examine the dose–response relation between energy level and cardioversion success by electrode position in elective cardioversion.

**Methods** We searched PubMed, Embase, The Cochrane Library, Google Scholar and Scopus Citations. Inclusion criteria were randomised controlled trials using biphasic shock waves and self-adhesive patches, and publication date from 2000 to 2023. We used random-effects dose-response models to meta-analyse the relation between energy level and cardioversion success by anterolateral and anteroposterior position. Random-effects models estimated pooled risk ratios (RR) for cardioversion success after the first and the final shocks between the two electrode positions.

**Results** We included five randomised controlled trials (N=1078). After the first low-energy shock, the electrode position was not significantly associated with the likelihood of successful cardioversion (pooled RR anterolateral vs anteroposterior placement 1.28, 95% CI 0.93 to 1.76, with considerable heterogeneity). After a high-energy final shock, there was no evidence of an association between the electrode position and the cumulative chance of cardioversion success (pooled RR anterolateral vs anteroposterior 1.05, 95% CI 0.97 to 1.14). Regardless of electrode position, cardioversion success was significantly less likely with shock energy levels < 200J compared with 200J.

**Conclusion** Evidence from contemporary randomised trials suggests that higher level of electrical energy is associated with higher conversion rate when cardioverting AF with a biphasic shockwave. Positioning of electrodes can be based on convenience.

## INTRODUCTION

Atrial fibrillation (AF) is the most common sustained arrhythmia in clinical practice, with a lifetime risk of one in three.<sup>1</sup> In contemporary practice, patients with incident AF lose on average 2 years of expected lifetime over 10 years of follow-up.<sup>2</sup> Rhythm

## WHAT IS ALREADY KNOWN ON THIS TOPIC

- ⇒ Several systematic reviews with meta-analyses of randomised controlled trials that examined the optimal electrode position for cardioverting atrial fibrillation have shown conflicting results.
- ⇒ Attention has increasingly been focused on the electrical energy delivered and the success rate of electrical cardioversion, but this has been analysed sparsely in meta-analysis.

## WHAT THIS STUDY ADDS

- ⇒ Applied energy levels below 200J were significantly associated with lower chances of success compared with energy applied at 200J, while there was no evidence of differential cardioversion success between energy levels above 200J.
- ⇒ There were no substantial differences between the two electrode positions, although with considerable heterogeneity.

## HOW THIS STUDY MIGHT AFFECT RESEARCH, PRACTICE OR POLICY

- ⇒ This systematic review with meta-analysis of biphasic shock and self-adhesive electrodes suggests that shock energy is more important for effective electrical cardioversion than the electrode position.
- ⇒ The electrode placement may depend on the physician's discretion.

control constitutes a central part of symptom management in the Atrial fibrillation Better Care pathway for integrated care.<sup>3</sup> Elective electrical cardioversion is often used for rhythm control of AF and has a high immediate success rate for restoring normal sinus rhythm, but the intermediate-term and long-term recurrence rates are high.<sup>4,5</sup>

The current European Society of Cardiology (ESC) guidelines include no specific guidance on the electrode position.<sup>3</sup> Yet, more systematic reviews with meta-analyses of randomised controlled trials (RCTs) have recently examined the optimal electrode position for cardioverting AF, but the results are conflicting.<sup>6–11</sup> Lately, attention has



© Author(s) (or their employer(s)) 2023. Re-use permitted under CC BY-NC. No commercial re-use. See rights and permissions. Published by BMJ.

For numbered affiliations see end of article.

## Correspondence to

Dr Nicklas Vinter; [nicvin@rm.dk](mailto:nicvin@rm.dk)

increasingly been focused on the electrical energy delivered and the success rate of electrical cardioversion.<sup>12</sup> Systematic reviews with meta-analysis have sparsely analysed the association between energy dose and effect,<sup>7,9</sup> and the ESC guidelines for AF do not state any recommendations on the most effective strategy.<sup>3</sup>

In this study, we performed a systematic review and meta-analysis of the dose–response relation between applied energy and cardioversion rates. As patch position may influence the success rate of electrical cardioversion, we included RCTs that examined self-adhesive patches positioned anterior lateral (AL) or anterior–posterior. The review adhered to the Preferred Reporting Items for Systematic Reviews and Meta-Analyses (PRISMA) 2020 statement.<sup>13</sup>

## METHODS

### Eligibility criteria

We selected RCTs that used a step-up protocol using increasing electrical current and compared anterolateral vs anteroposterior electrode placement for elective cardioversion of AF among adults (>18 years of age) published from 2000 to 2023. Eligible RCTs were required to use self-adhesive patch electrodes and biphasic shockwave to reflect contemporary practice. Trials that reported use of monophasic shockwaves or manual hand-held paddles were not eligible for the reason of not being a standard procedure in contemporary medical practice. The RACE 7 study reported that in patients presenting to the emergency department with recent-onset and symptomatic AF, a wait-and-see approach was non-inferior to early cardioversion in achieving a return to sinus rhythm at 4 weeks.<sup>14</sup> Therefore, we did not include studies reporting on acute cardioversions in this systematic review. We intended to select articles published in English, Spanish, Portuguese, Danish, Norwegian or Swedish. This review was not registered.

### Search strategy and information sources

We searched PubMed, Embase and the Cochrane Library from 2000 up to and including 2023. The final search was performed on 18 July 2023. The search strategy is reported in online supplemental table 1. We developed the search strategy with the help of a professional healthcare librarian. To account for publications not indexed in the three databases, Scopus Citations and Google Scholar were searched. All potential records were manually screened for eligibility. Two reviewers assessed each record for inclusion based on titles and abstracts. Eligible articles were retrieved as full-text and read by two independent reviewers (LF and NV). Discrepancies were resolved by formal consensus. Finally, we screened the list of references of selected studies.

### Data collection process

Two reviewers extracted all data independently and in duplicate. We evaluated study characteristics, including trial location, whether patients with recent-onset or

persistent AF were included, inclusion and exclusion criteria, and the shock protocol (energy level of shocks and step-up protocol). We also assessed patient characteristics, including mean age, mean body mass index, proportion of men and proportion of patients with hypertension.

We examined restoration of sinus rhythm by delivered energy (dose–response evaluation). The outcomes of interest were restoration of sinus rhythm after the first shock in a step-up protocol using increasing electrical current, and restoration of sinus rhythm after the final shock. The final shock was either the shock that led to restoration of sinus rhythm or the final shock in the study-specific shock protocol. From each study, we collected the total number of patients and the number of patients with restored sinus rhythm after the first shock and after all consecutive shocks. We extracted the outcome data for success as defined according to each study-specific protocol (table 1). Some RCTs used a step-up protocol, which included sequential shocks with increasing energy and a final cross-over of electrodes (switching from the initial allocated position to the alternate position on cardioversion failure). In studies with cross-over protocols, we considered the final shock as the last one in the allocated electrode position and not after cross-over. Trial investigators were contacted to obtain missing data. In Muñoz-Martínez *et al's* study,<sup>15</sup> we used the first of two shocks with 200J for the dose–response analysis.

### Assessment of risk of bias

Reviewers assessed within-study biases with the RoB 2 Tool (version 2 of the Cochrane risk-of-bias tool for randomised trials).<sup>16</sup> This tool provided a framework for the assessment of the overall risk of bias by evaluating: (1) the randomisation process, (2) deviations from the intended procedure, (3) missing outcome data, (4) measurement of outcome and (5) selective reporting. To assess small-study effects, we created funnel plots for the first and final shock conversion success outcomes.

### Synthesis methods

We calculated the cumulative proportions of patients with restored sinus rhythm by cumulative shocks and estimated risk ratios (RRs). For example, when counting patients with restored sinus rhythm after the second shock, patients with restored sinus rhythm after both the first and second shock were included in the numerator and all patients were included in the denominator. The RRs were pooled across eligible studies by using inverse-variance random-effects models. We used the Paule-Mandel procedure to estimate the between-trial variance with the Knapp-Hartung adjustment procedure. To quantify heterogeneity between studies, we also estimated the  $I^2$  statistic. To examine the effect of shock energy, we conducted a dose–response meta-analysis to assess the association of shock energy with the probability of restored sinus rhythm, for each electrode position separately. In each study, we extracted the cumulative number

**Table 1** Study characteristics

Reference	Location	Sample size	Recent onset or persistent AF	Inclusion criteria	Exclusion criteria	Shock protocol suggests	Successful cardioversion
Walsh <i>et al</i> 2005 <sup>25</sup>	England	294	Persistent	Elective cardioversion of stable AF	Other arrhythmias, electrolyte imbalances or age <18 years	70, 100, 150, 200J	Restoration of sinus rhythm for at least 30 s after a shock
Siaplaouras <i>et al</i> 2005 <sup>23</sup>	Germany	123	Persistent	Elective cardioversion of stable AF	Other arrhythmias, pacemaker, potassium <3.5 or >5 mmol/L	120, 150, 200J	Termination of AF with at least two consecutive sinus beats after a shock
Brazdionyte <i>et al</i> 2006 <sup>24</sup>	Lithuania	103	Recent onset/persistent	Elective cardioversion of stable AF	Age <18 years. Inadequate anticoagulation therapy*	100, 150, 200, 300J+crossover	Presence of at least one clearly visible P wave within 30 s after the administration of the shock
Muñoz-Martínez <i>et al</i> 2010 <sup>15</sup>	Spain	91	Persistent	Elective cardioversion of persistent and stable AF	Age <18 years, acute myocardial infarction, pregnancy, high risk of thromboembolism†	150, 200, 200J+crossover‡	After the final shock all patients were observed for 15 min at the intensive care unit and then moved back to the department and discharged with sinus rhythm after 2 hours if the patient was stable.
Schmidt <i>et al</i> 2021 <sup>26</sup>	Denmark	467	Recent onset/persistent	Elective cardioversion of stable AF	Age <18 years, other arrhythmias, ICD, pregnancy or previous enrollment in protocol	100, 150, 200, 360J	Sinus rhythm 1 min after first shock or 1 min after final shock.

\*International normalised ratio >2 for at least 3 weeks before cardioversion.  
†Inadequate anticoagulation therapy or verified auricular thrombus in echocardiography.  
‡As the energy level for second and third shock were similar, we counted the second shock as the final.  
AF, atrial fibrillation; ICD, implantable cardioverter-defibrillator.

of patients with restored sinus rhythm at each increasing energy level; we assumed that patients with success at lower energy levels would have success at a given energy level. We fitted a one-stage random-effects dose–response model using restricted cubic splines with three knots for each electrode position.<sup>17</sup> As all studies delivered a 200J shock, this amount of energy was used as the reference level in this analysis.

All analyses were performed in R V.4.0.3., with the ‘meta’ package, except the dose–response model that we fitted with Stata V.15.1 by using the command `drmeta`.

## RESULTS

### Literature search

Online supplemental figure 1 shows the flow of study selection. The initial search yielded 331 results. We retrieved 10 full-text records of which five studies were excluded because of monophasic shock use

and/or use of hand-held defibrillator paddles.<sup>18–22</sup> We included five RCTs,<sup>15 23–26</sup> with a total of 1078 patients. Of the patients, 547 were allocated to the AL electrode placement, and 531 patients were allocated to the anterior–posterior electrode placement.

### Trial and baseline patient characteristics

The five trials included ‘recent-onset’ (AF present <48 hours) or persistent AF. The mean age of participants ranged from 55 to 69 years, the proportion of men ranged from 63% to 82.5%, and the prevalence of hypertension from 32% to 64.5% (table 2).

The trials used different step-up protocols with sequential shocks of increasing energy (tables 1 and 3). Two trials included a cross-over shock with high energy.<sup>15 24</sup> The anterior–posterior electrode position differed between trials, with some placing the electrodes in the left infraclavicular and left infrascapular

**Table 2** Baseline characteristics of study populations in included trials

Trial	Sample size		Age (years)		Sex, male		Body mass index (kg/m <sup>2</sup> )		Hypertension	
	AL	AP	AL	AP	AL	AP	AL	AP	AL	AP
Siaplaouras <i>et al</i> <sup>23</sup> 2005	63	60	66±10	67±10	47 (75)	40 (67)	28±5	28±4	18 (28)	26 (44)
Walsh <i>et al</i> <sup>25</sup> 2005	150	144	67±10	66±14	95 (63)	100 (64)	28±5	29±5	57 (38)	81 (52)
Brazdzionyte <i>et al</i> <sup>24</sup> 2006	55	48	63±12	62±10	36 (66)	29 (60)	30±5	30±5	20 (36)	19 (39)
Muñoz-Martínez <i>et al</i> <sup>15</sup> 2010	46	45	63±9	55±13	40 (87)	35 (78)	NA	NA	15 (33)	14 (31)
Schmidt <i>et al</i> <sup>26</sup> 2021	233	234	69±10	69±9	156 (67)	158 (67)	29±6	29±5	149 (64)	151 (65)

Data are mean ±SD or n (%).  
AL, anterior lateral; AP, anterior–posterior; NA, not available.

region,<sup>15 24 26</sup> while others used the right infraclavicular and left infrascapular region,<sup>25</sup> and one trial placed the electrodes in the midsternal and interscapular region.<sup>23</sup>

In all RCTs, clinicians and patients were not blinded, and only one study used blinded adjudication of the outcome.<sup>26</sup> The outcome definition differed between trials, one trial defined successful cardioversion as two consecutive P waves within 1 min after the procedure,<sup>23</sup> another trial defined cardioversion as restoration of sinus rhythm for a least 30 s,<sup>25</sup> one trial defined success as at least one clearly visible P wave within 30 s after the shock,<sup>24</sup> and another trial defined the outcome as sinus rhythm 1 min after the final

shock.<sup>26</sup> One trial did not specify the time window for the adjudication of successful cardioversion.<sup>15</sup>

### Effect of energy level by electrode position

After a first low-energy shock, the electrode position was not significantly associated with the likelihood of successful cardioversion (pooled RR for anterolateral vs anteroposterior position: 1.28, 95% CI 0.93 to 1.76, with considerable heterogeneity across trials, figure 1). After a high-energy final shock as per protocol, we found no evidence of a difference between the two electrode positions (pooled RR for anterolateral vs anteroposterior electrode position: 1.05, 95% CI 0.97 to 1.14). We

**Table 3** Dose–response evaluation of cumulated cardioversion proportion of biphasic electrical cardioversion of atrial fibrillation using self-adhesive patches in anterolateral versus anteroposterior positions

Energy (J)	Trial	Anterolateral cardioversion proportion	Anteroposterior cardioversion proportion
70	Walsh <i>et al</i> <sup>25</sup> 2005	54/150	45/144
100	Walsh <i>et al</i> <sup>25</sup> 2005	99/150	74/144
	Brazdzionyte <i>et al</i> <sup>24</sup> 2006	40/55	29/48
	Schmidt <i>et al</i> <sup>26</sup> 2021	126/233	77/234
120	Siaplaouras <i>et al</i> <sup>23</sup> 2005	47/63	47/60
150	Siaplaouras <i>et al</i> <sup>23</sup> 2005	55/63	54/60
	Walsh <i>et al</i> <sup>25</sup> 2005	123/150	109/144
	Brazdzionyte <i>et al</i> <sup>24</sup> 2006	52/55	41/48
	Muñoz-Martínez <i>et al</i> <sup>15</sup> 2010*	32/46	18/45
	Schmidt <i>et al</i> <sup>26</sup> 2021	175/233	125/234
200	Siaplaouras <i>et al</i> <sup>23</sup> 2005	60/63	57/60
	Walsh <i>et al</i> <sup>25</sup> 2005	143/150	127/144
	Brazdzionyte <i>et al</i> <sup>24</sup> 2006	53/55	46/48
	Muñoz-Martínez <i>et al</i> <sup>15</sup> 2010, first shock*	39/46	27/45
	Muñoz-Martínez <i>et al</i> <sup>15</sup> 2010, second shock	41/46	32/45
300	Schmidt <i>et al</i> <sup>26</sup> 2021	200/233	162/234
360	Brazdzionyte <i>et al</i> <sup>24</sup> 2006	54/55	47/48
	Schmidt <i>et al</i> <sup>26</sup> 2021	216/233	200/234


\*Data shared by the author. In the dose–response analyses, we used the first of the two shocks.



**First shock**

Study	AL		AP		Weight	Risk Ratio IV, Random, 95% CI
	Events	Total	Events	Total		
Siaplaouras 2005	47	63	47	60	23.9%	0.95 [0.78; 1.16]
Walsh 2005	54	150	45	144	18.2%	1.15 [0.83; 1.59]
Brazdzionyte 2006	40	55	29	48	20.1%	1.20 [0.91; 1.59]
Schmidt 2021	126	233	77	234	22.9%	1.64 [1.32; 2.04]
Muñoz 2010	32	46	18	45	14.9%	1.74 [1.16; 2.61]
<b>Total (95% CI)</b>	<b>547</b>		<b>531</b>		<b>100.0%</b>	<b>1.28 [0.93; 1.76]</b>


Heterogeneity: Tau<sup>2</sup> = 0.0443; Chi<sup>2</sup> = 16.29, df = 4 (P < 0.01); I<sup>2</sup> = 75%

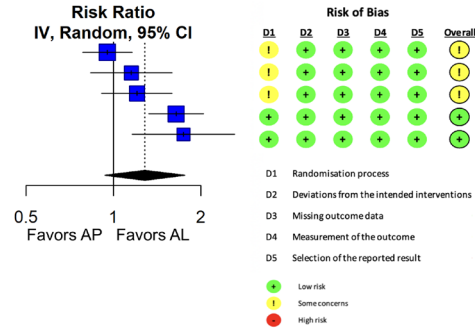

**Final shock**

Study	AL		AP		Weight	Risk Ratio IV, Random, 95% CI
	Events	Total	Events	Total		
Siaplaouras 2005	60	63	57	60	20.5%	1.00 [0.93; 1.09]
Brazdzionyte 2006	54	55	47	48	26.4%	1.00 [0.95; 1.06]
Walsh 2005	143	150	127	144	22.9%	1.08 [1.01; 1.16]
Schmidt 2021	216	233	200	234	24.2%	1.08 [1.02; 1.16]
Muñoz 2010	41	46	32	45	5.9%	1.25 [1.01; 1.55]
<b>Total (95% CI)</b>	<b>547</b>		<b>531</b>		<b>100.0%</b>	<b>1.05 [0.97; 1.14]</b>

Heterogeneity: Tau<sup>2</sup> = 0.0023; Chi<sup>2</sup> = 8.26, df = 4 (P = 0.08); I<sup>2</sup> = 52%

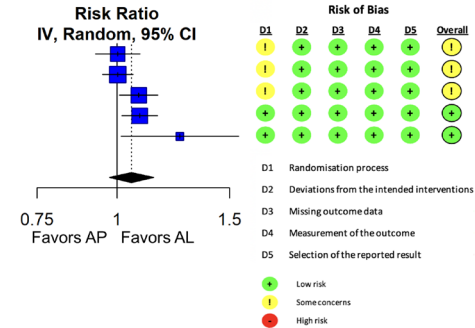


**Figure 1** Meta-analysis comparing electrode pad position at first shock and final shock. AL, anterior lateral; AP, anterior-posterior; IV, inverse variance.

found a dose-response association so that an increasing shock energy was associated with a higher probability of cardioversion success to sinus rhythm (figure 2). Applied energy levels below 200J were significantly associated with lower chances of success compared with energy applied at 200J. Conversely, there was no evidence of differential cardioversion success between energy levels above 200J

and at 200J. We found no substantial differences between the two electrode positions.

Figure 1 shows the risk of bias assessment across trials. Two studies had some concerns, and no study was deemed at high risk of bias. We did not find any indication of small-study effects on either outcome after the first or final shock, although the number of studies was

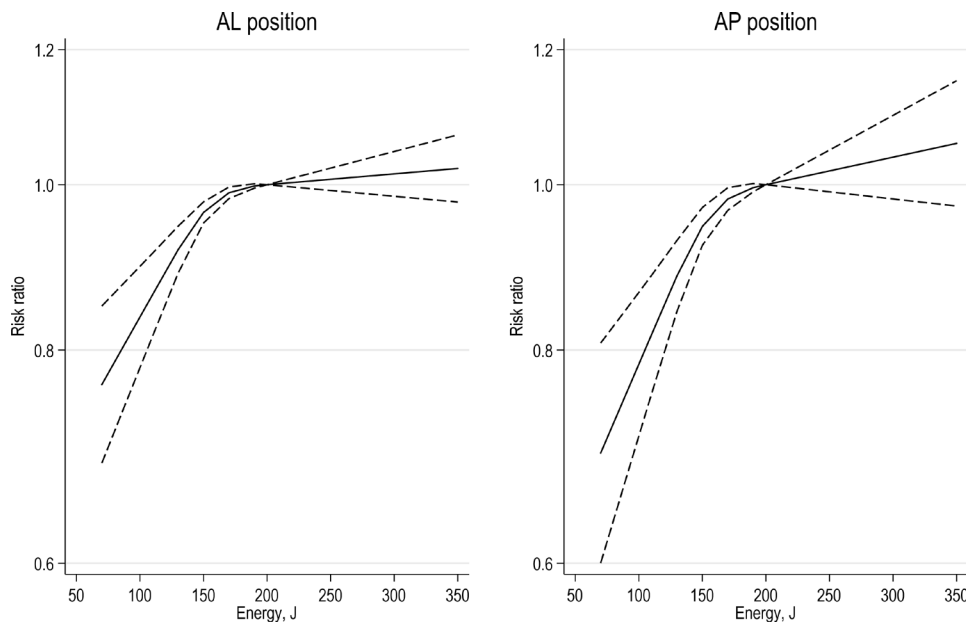

**Figure 2** Dose-response relationship between biphasic shock energy (Joule) and successful cardioversion using anterolateral and anteroposterior self-adhesive patch position. For AL and AP separately, each figure shows risk ratios for restored sinus rhythm between the shock energy level on the horizontal axis and 200 J (as a reference), together with 95% CIs. AL, anterior lateral; AP, anterior-posterior.

small for interpreting the funnel plots (online supplemental figure 1).

## DISCUSSION

This comprehensive systematic review that included a meta-analysis and dose–response evaluation presents an up-to-date analysis of RCTs that compared anterolateral versus anteroposterior electrode positioning in cardioversion of AF using biphasic shock and self-adhesive electrodes. The results showed that applied energy levels below 200J were significantly associated with lower chances of success compared with energy applied at 200J, while there was no evidence of differential cardioversion success between energy levels above 200J. We found no substantial differences between the two electrode positions, although with considerable heterogeneity.

Recently, a systematic review with meta-analyses by Nguyen *et al* examined cardioversion success, electrode position and energy level, respectively.<sup>7</sup> We aimed to examine the relationship between energy level and cumulative cardioversion success. In contrast, Nguyen *et al* aimed to compare the cumulative cardioversion success between high-energy shocks (minimum 200J) and escalating energy protocols. Our prespecified eligibility criteria focused on trials that randomised electrode placement and that used biphasic shock waves while trials of acute cardioversion or those involving monophasic shockwaves or manual hand-held paddles that no longer reflect standard contemporary practice were not eligible. Our meta-analysis included five randomised trials, none of which overlapped with the four randomised trials selected by Nguyen *et al*. Nguyen *et al* reported that high-energy shocks did not significantly improve cumulative cardioversion success compared with an escalating energy protocol. A subgroup analysis suggested a larger effect with anteroposterior pad positioning compared with anteroapical or anterolateral positioning. In contrast, we found a dose–response relationship with increasing levels of energy leading to larger cardioversion success rate up to 200J. Beyond 200J, we found no evidence of improved cardioversion success. Additionally, we found no evidence of difference between anteroposterior and anterolateral pad positioning.

Assessment of risk of bias of the included trials showed some concerns in two trials. Four out of five trials did not report any method for allocation concealment, which may increase the risk of selection bias. Due to the nature of the studies, blinding of personnel and trialists was impossible, though the open-label design was not thought to influence the outcome assessment. Only one trial had blinded outcome adjudication,<sup>26</sup> and only two trials were rated as having low risk of bias.

Participants in the included studies differed with respect to age, weight, comorbidities, duration of AF and use of antiarrhythmics drugs. For example, the user rate of amiodarone varied from 9% to 10% in one trial<sup>25</sup> to from 40% to 50% in another trial.<sup>24</sup> Such factors are known

to influence the cardioversion rate. Selected studies used slightly different methods to ascertain success as well as different step-up protocols with initial low-energy shock, the latter not being in line with contemporary practice. Furthermore, electrode placement, specifically the anteroposterior electrode placement, was slightly different (eg, right infraclavicular or left infraclavicular) between the trials. Differences in anteroposterior position could, theoretically, target the atrium differently and therefore be of significance in cardioversion success. Only 4% of the transthoracic shock traverses the heart while the rest of the current is shunted around the heart and through the thoracic cage and lungs.<sup>27</sup> Therefore, a successful cardioversion could be more dependent on the total energy delivery rather than electrode placement, a trend that was observed in all RCTs.

Schmidt *et al* showed that adverse events, for example, arrhythmias and transient bradycardia, were rare.<sup>26</sup> Other adverse effects such as skin discomfort was rarely experienced.<sup>26</sup> A recent study by Lobo *et al* examined the effect of high-energy biphasic shock cardioversion on high-sensitive troponin release, and even when delivering 360J shocks, an increase in troponin release could not be detected; hence, cardioversion should be considered a safe procedure, even at high energy shock delivery.<sup>28</sup> One randomised trial demonstrated that maximum fixed energy shocks of 360J had higher conversion rates compared with sequential and escalating shock energies.<sup>12</sup> However, considering the high conversion rates at 200J, independent of electrode position, it can be speculated that electrode position becomes irrelevant when delivering high energy shocks ( $\geq 200$ J).

## Limitations

This meta-analysis included five relatively small studies and has, therefore, limited statistical power and precision. There was considerable clinical diversity across studies, which resulted in large statistical heterogeneity. Studies were non-blinded, and outcome assessment was blinded in only one study. Results from our dose–response analyses should be interpreted with caution given the risk of ecological bias and considerable clinical diversity across studies. Moreover, we made the assumption that success at a lower energy level would have been observed at a higher energy level.

## CONCLUSIONS

This systematic review and meta-analysis of contemporary RCTs suggest that an initial shock energy of 200J, possibly followed by higher energy shocks up to 360J, has a higher success than previously used lower energy shocks when elective cardioverting AF. We did not find evidence of differential success between anterolateral and anteroposterior electrode positions, although with considerable heterogeneity across trials. These findings suggest that the electrode position is not a critical factor compared with shock energy, and the placement may depend on

the physician's discretion, with possible preference for AL placement.

#### Author affiliations

<sup>1</sup>Diagnostic Centre, Silkeborg Regional Hospital, Silkeborg, Denmark

<sup>2</sup>Department of Clinical Medicine, Aalborg University, Aalborg, Denmark

<sup>3</sup>Danish Center for Health Services Research, Department of Clinical Medicine, Aalborg University, Aalborg, Denmark

<sup>4</sup>Liverpool Centre of Cardiovascular Science at University of Liverpool, Liverpool John Moores University and Liverpool Heart & Chest Hospital, Liverpool, UK

<sup>5</sup>Tufts Clinical and Translational Science Institute, Tufts University, Boston, Massachusetts, USA

<sup>6</sup>Institute for Clinical Research and Health Policy Studies, Tufts Medical Center, Boston, Massachusetts, USA

**Twitter** Nicklas Vinter @nicklas\_vinter

**Contributors** NV, LF, MZBH-H and LT: conceptualisation, methodology and writing-original draft preparation. LF and LT: supervision and investigation. NV, LF and MZBH-H performed the searches and extracted data from the eligible studies. NV and MZBH-H assessed the quality of the studies, and NV conducted the statistical analysis with critical appraisal from LT. NV led the drafting of the manuscript, with review and contributions from LT, LF, MZBH-H, SPJ and GYHL. All authors contributed to the article and approved the submitted version. NV and LF are responsible for the overall content as guarantor.

**Funding** The authors have not declared a specific grant for this research from any funding agency in the public, commercial or not-for-profit sectors.

**Competing interests** NV: Grants from the Danish Cardiovascular Academy, the Health Research Foundation of Central Denmark Region, and the Danish Heart Foundation. Advisory board member for Astra Zeneca. No fees were received personally. MZBH-H: none declared SPJ: Consultant and speaker for BMS/Pfizer. Research grants from BMS/Pfizer and Novo Nordisk. GYHL: Consultancy and speaker fees from BMS/Pfizer, Boehringer Ingelheim and Daiichi-Sankyo outside the submitted work. No fees received personally. LF: Supported by the Health Research Foundation of Central Denmark Region. Consultant for BMS and Pfizer. LT: Received funding from the American Heart Association (18SFRN34150007)

**Patient consent for publication** Not applicable.

**Provenance and peer review** Not commissioned; externally peer reviewed.

**Data availability statement** All data relevant to the study are included in the article or uploaded as supplementary information.

**Supplemental material** This content has been supplied by the author(s). It has not been vetted by BMJ Publishing Group Limited (BMJ) and may not have been peer-reviewed. Any opinions or recommendations discussed are solely those of the author(s) and are not endorsed by BMJ. BMJ disclaims all liability and responsibility arising from any reliance placed on the content. Where the content includes any translated material, BMJ does not warrant the accuracy and reliability of the translations (including but not limited to local regulations, clinical guidelines, terminology, drug names and drug dosages), and is not responsible for any error and/or omissions arising from translation and adaptation or otherwise.

**Open access** This is an open access article distributed in accordance with the Creative Commons Attribution Non Commercial (CC BY-NC 4.0) license, which permits others to distribute, remix, adapt, build upon this work non-commercially, and license their derivative works on different terms, provided the original work is properly cited, appropriate credit is given, any changes made indicated, and the use is non-commercial. See: <http://creativecommons.org/licenses/by-nc/4.0/>.

#### ORCID iDs

Nicklas Vinter <http://orcid.org/0000-0003-0558-8483>

Søren Paaske Johnsen <http://orcid.org/0000-0002-2787-0271>

Gregory Y H Lip <http://orcid.org/0000-0002-7566-1626>

Lars Frost <http://orcid.org/0000-0001-9215-9796>

Ludovic Trinquart <http://orcid.org/0000-0002-3028-4900>

#### REFERENCES

- 1 Staerk L, Wang B, Preis SR, *et al*. Lifetime risk of atrial fibrillation according to optimal, borderline, or elevated levels of risk factors: cohort study based on longitudinal data from the framingham heart study. *BMJ* 2018;361:k1453.
- 2 Vinter N, Huang Q, Fenger-Grøn M, *et al*. Trends in excess mortality associated with atrial fibrillation over 45 years (Framingham heart study): community based cohort study. *BMJ* 2020;370:m2724.
- 3 Hindricks G, Potpara T, Dagres N, *et al*. ESC guidelines for the diagnosis and management of atrial fibrillation developed in collaboration with the European Association for Cardio-Thoracic surgery (EACTS): the task force for the diagnosis and management of atrial fibrillation of the European society of cardiology (ESC) developed with the special contribution of the European Heart Rhythm Association (EHRA) of the ESC. *Eur Heart J* 2020;42:373–498.
- 4 Brandes A, Crijns H, Rienstra M, *et al*. Cardioversion of atrial fibrillation and atrial flutter revisited: current evidence and practical guidance for a common procedure. *Europace* 2020;22:1149–61.
- 5 Vinter N, Frederiksen AS, Albertsen AE, *et al*. Role for machine learning in sex-specific prediction of successful electrical cardioversion in atrial fibrillation? *Open Heart* 2020;7:e001297.
- 6 Motawea KR, Mostafa MR, Aboelenen M, *et al*. Anterolateral versus anterior-posterior electrodes in external cardioversion of atrial fibrillation: a systematic review and meta-analysis of clinical trials. *Clin Cardiol* 2023;46:359–75.
- 7 Nguyen ST, Belley-Côté EP, Ibrahim O, *et al*. Techniques improving electrical cardioversion success for patients with atrial fibrillation: a systematic review and meta-analysis. *Europace* 2023;25:318–30.
- 8 Eid M, Abu Jazar D, Medhekar A, *et al*. Anterior-posterior versus anterior-lateral electrode position for electrical cardioversion of atrial fibrillation: a meta-analysis of randomized controlled trials. *Int J Cardiol Heart Vasc* 2022;43:101129.
- 9 Virk SA, Rubenis I, Brieger D, *et al*. Anteroposterior versus anterolateral electrode position for direct current cardioversion of atrial fibrillation: a meta-analysis of randomised controlled trials. *Heart Lung Circ* 2022;31:1640–8.
- 10 Salah HM, Devabhaktuni SR, Shah SD, *et al*. Meta-analysis comparing anterior-lateral versus anterior-posterior electrode position for biphasic cardioversion in atrial fibrillation. *Am J Cardiol* 2022;169:164–5.
- 11 Kirkland S, Stiell I, AlShawabkeh T, *et al*. The efficacy of pad placement for electrical cardioversion of atrial fibrillation/flutter: a systematic review. *Acad Emerg Med* 2014;21:717–26.
- 12 Schmidt AS, Lauridsen KG, Torp P, *et al*. Maximum-fixed energy shocks for cardioverting atrial fibrillation. *Eur Heart J* 2020;41:626–31.
- 13 Page MJ, McKenzie JE, Bossuyt PM, *et al*. The PRISMA 2020 statement: an updated guideline for reporting systematic reviews. *BMJ* 2021;372:71.
- 14 Pluymaekers N, Dudink E, Crijns H. Early or delayed cardioversion in recent-onset atrial fibrillation. reply. *N Engl J Med* 2019;381:387–8.
- 15 Muñoz-Martínez T, Castañeda-Saiz A, Vinuesa-Lozano C, *et al*. Electrode position in elective electrical cardioversion of atrial fibrillation: a randomized study. *Med Intensiva* 2010;34:225–30.
- 16 Sterne JAC, Savović J, Page MJ, *et al*. Rob 2: a revised tool for assessing risk of bias in randomised trials. *BMJ* 2019;366:l4898.
- 17 Shim SR, Lee J. Dose-response meta-analysis: application and practice using the R software. *Epidemiol Health* 2019;41:e2019006.
- 18 Kirchhof P, Eckardt L, Loh P, *et al*. Anterior-posterior versus anterior-lateral electrode positions for external cardioversion of atrial fibrillation: a randomised trial. *Lancet* 2002;360:1275–9.
- 19 Chen C-J, Guo G-F. External cardioversion in patients with persistent atrial fibrillation: a reappraisal of the effects of electrode pad position and transthoracic impedance on cardioversion success. *Jpn Heart J* 2003;44:921–32.
- 20 Alp NJ, Rahman S, Bell JA, *et al*. Randomised comparison of antero-lateral versus antero-posterior paddle positions for DC cardioversion of persistent atrial fibrillation. *Int J Cardiol* 2000;75:211–6.
- 21 Vogiatzis IA, Sachpekidis V, Vogiatzis IM, *et al*. External cardioversion of atrial fibrillation: the role of electrode position on cardioversion success. *Int J Cardiol* 2009;137:e8–10.
- 22 Stanaitiene G, Babarskiene RM. Impact of electrical shock waveform and paddle positions on efficacy of direct current cardioversion for atrial fibrillation. *Medicina (Kaunas)* 2008;44:665–72.
- 23 Siaplaouras S, Buob A, Rötter C, *et al*. Randomized comparison of anterolateral versus anteroposterior electrode position for biphasic external cardioversion of atrial fibrillation. *Am Heart J* 2005;150:150–2.
- 24 Brazdzionyte J, Babarskiene RM, Stanaitiene G. Anterior-posterior versus anterior-lateral electrode position for biphasic cardioversion of atrial fibrillation. *Medicina (Kaunas)* 2006;42:994–8.



- 25 Walsh SJ, McCarty D, McClelland AJJ, *et al.* Impedance compensated biphasic waveforms for transthoracic cardioversion of atrial fibrillation: a multi-centre comparison of antero-apical and Antero-posterior pad positions. *Eur Heart J* 2005;26:1298–302.
- 26 Schmidt AS, Lauridsen KG, Møller DS, *et al.* Anterior-lateral versus anterior-posterior electrode position for cardioverting atrial fibrillation. *Circulation* 2021;144:1995–2003.
- 27 Lerman BB, Deale OC. Relation between transcardiac and transthoracic current during defibrillation in humans. *Circ Res* 1990;67:1420–6.
- 28 Lobo R, Jaffe AS, Cahill C, *et al.* Significance of high-sensitivity troponin T after elective external direct current cardioversion for atrial fibrillation or atrial flutter. *Am J Cardiol* 2018;121:188–92.