



Aalborg Universitet

AALBORG UNIVERSITY  
DENMARK

## Measurement Capabilities and Equipment at the Building Material Characterization Laboratory of Aalborg University (2024)

Johra, Hicham

DOI (link to publication from Publisher):  
[10.54337/aau580248093](https://doi.org/10.54337/aau580248093)

Creative Commons License  
CC BY 4.0

Publication date:  
2023

Document Version  
Publisher's PDF, also known as Version of record

[Link to publication from Aalborg University](#)

Citation for published version (APA):  
Johra, H. (2023). *Measurement Capabilities and Equipment at the Building Material Characterization Laboratory of Aalborg University (2024)*. Department of the Built Environment, Aalborg University. DCE Latest News No. 60 <https://doi.org/10.54337/aau580248093>

### General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal -

### Take down policy

If you believe that this document breaches copyright please contact us at [vbn@aub.aau.dk](mailto:vbn@aub.aau.dk) providing details, and we will remove access to the work immediately and investigate your claim.



DEPARTMENT OF THE BUILT ENVIRONMENT  
AALBORG UNIVERSITY

# Measurement Capabilities and Equipment at the Building Material Characterization Laboratory of Aalborg University (2024)

Hicham Johra





Aalborg University  
Department of the Built Environment  
Division of Sustainability, Energy & Indoor Environment

**DCE Latest News No. 60**

**Measurement Capabilities and Equipment  
at the Building Material Characterization  
Laboratory of Aalborg University (2024)**

by

Hicham Johra

November 2023

© Aalborg University

## **Scientific Publications at the Department of the Built Environment**

**Technical Reports** are published for timely dissemination of research results and scientific work carried out at the Department of the Built Environment at Aalborg University. This medium allows publication of more detailed explanations and results than typically allowed in scientific journals.

**Technical Memoranda** are produced to enable the preliminary dissemination of scientific work by the personnel of the Department of the Built Environment where such release is deemed to be appropriate. Documents of this kind may be incomplete or temporary versions of papers—or part of continuing work. This should be kept in mind when references are given to publications of this kind.

**Contract Reports** are produced to report scientific work carried out under contract. Publications of this kind contain confidential matter and are reserved for the sponsors and the Department of the Built Environment. Therefore, Contract Reports are generally not available for public circulation.

**Lecture Notes** contain material produced by the lecturers at the Department of the Built Environment for educational purposes. This may be scientific notes, lecture books, example problems or manuals for laboratory work, or computer programs developed at the Department of the Built Environment.

**Theses** are monographs or collections of papers published to report the scientific work carried out at the Department of the Built Environment to obtain a degree as either PhD or Doctor of Technology. The thesis is publicly available after the defence of the degree.

**Latest News** is published to enable rapid communication of information about scientific work carried out at the Department of the Built Environment. This includes the status of research projects, developments in the laboratories, information about collaborative work and recent research results.

Published 2023 by  
Aalborg University  
Department of the Built Environment  
Thomas Manns Vej 23  
DK-9220 Aalborg Ø, Denmark

Printed in Aalborg at Aalborg University

ISSN 1901-7308  
DCE Latest News No. 60

## Contents

1. Foreword .....	6
2. Physical Properties .....	7
2.1. Density, Mass and Volume .....	7
3. Heat Transport and Dynamics Properties .....	8
3.1. Thermal Conductivity .....	8
3.2. Specific Heat Capacity .....	11
3.3. Thermal Diffusivity.....	14
4. Air transport properties.....	15
4.1. Effective Air Permeability .....	15
4.2. Gas Diffusion Coefficient .....	16
5. Moisture Transport and Dynamics Properties .....	17
5.1. Hygrothermal Properties: Water Vapor Sorption and Desorption Capacity.....	17
5.2. Gas Diffusion Coefficient .....	18
5.3. Water Vapor Permeability .....	19
5.3. Humidity Content .....	20
References .....	21

## **1. Foreword**

The aim of this short communication report is to provide synthetic information concerning the measurement capabilities and equipment of the Building Material Characterization Laboratory of Aalborg University - Department of the Built Environment [1]. This laboratory uses state-of-the-art equipment to determine the thermophysical properties and the heat-air-moisture transport characteristics of materials, especially construction materials.

## 2. Physical Properties

### 2.1. Density, Mass and Volume

The bulk density of material at room temperature and atmospheric pressure can rapidly be measured by assessing the volume (dimensions) of a sample with a precision ruler, a caliper or a micrometer, and the mass of that sample with a precision scale. For a very accurate measurement of the density of small-size samples (few millimeters or centimeters), one can use a specific experimental setup mounted on a precision scale and based on the Archimedes' principle of buoyancy [2].

- Precision **caliper** "Mitutoyo": measurement up to 300 mm; resolution 0.01 mm.
- Precision **micrometer** "Mitutoyo": measurement up to 25 mm; resolution 0.001 mm.
- Precision **scale** "Sartorius Entris": measurement up to 2200 g; resolution 0.01 g.
- Precision **scale** "Sartorius Entris" with protection glass enclosure: measurement up to 220 g; resolution 0.0001 g.
- Precision **scale** "Sartorius Cubis": measurement up to 5200 g; resolution 0.1 g.
- "Sartorius" **kit** for small-size sample density measurement with **Archimedes'** principle of buoyancy: sample diameter up to 40 mm.



**Figure 1:** Measurement of dimensions and volume with a precision caliper (left); accurate measurement of mass with a precision scale [3] (center); accurate measurement of the density of small-size samples with the Archimedes' principle of buoyancy on a precision scale [2] (right).



### 3. Heat Transport and Dynamics Properties

#### 3.1. Thermal Conductivity

The thermal conductivity of various types of material or entire construction elements can be measured with the appropriate equipment. The choice of the equipment mainly depends on the size of the sample to be tested: Small-size samples are tested with the Laser Flash Analysis Apparatus, medium-size samples are tested with the Guarded Hot Plate Apparatus [4], large full-scale construction elements are tested with the Guarded Hot Box, and very large full-scale construction elements are tested with the Big Guarded Hot Box. The smaller the sample the faster the measurement.

- **Laser Flash Analysis Apparatus LFA 447 [5] (see Figure 2):**
  - Thin sample of uniform thickness with smooth surfaces (no fibers or large pores structures).
  - Powder, liquid, slurry, layered material, graded material, anisotropic material.
  - Thermal conductivity range 0.1 – 2000 W/m.K.
  - Temperature range 10 – 300 °C.
  - Round sample of diameter 6 mm\*; 8 mm\*; 10 mm\*, 12.7 mm\*, 25.4 mm\*. Thickness 0.5 – 3 mm. \*can be diameter down to 1.2 mm less than prescribed diameter.
  - Scanning mode local measurement of large sample: round diameter 40 mm; square 50 x 50 mm. Resolution of 0.1 mm.
  - Measurement speed: ~ 3 min/measurement.




**Figure 2:** Laser Flash Analysis Apparatus LFA 447 (Netzsch Gerätebau GmbH) [5].

- **Guarded Hot Plate Apparatus EP500 [4][6] (see Figure 3):**
  - Cubical sample of uniform thickness with flat surfaces (compression of sample is controlled).
  - Thermal conductivity range 0.005 – 2 W/m.K.
  - Temperature range 10 – 40 °C.
  - Compression pressure range 0.05 - 2.5 kN/m<sup>2</sup> (5000 - 25000 Pa).
  - Sample dimension : 15 x 15 cm for conductive material, 50 x 50 cm for insulating material.
  - Sample thickness range 1 – 12 cm.
  - Measurement uncertainty always below 1 % and mostly below 0.5 %.
  - Measurement speed: ~ 5 hours/measurement.



- **Figure 3:** The Guarded Hot Plate Apparatus EP500 from Lambda-Messtechnik GmbH Dresden [6].

- **Guarded Hot Box** (see *Figure 4*):
  - Large full-scale vertical construction element.
  - Square element with dimensions ranging from 1 x 1 m to 2 x 2 m.
  - Thickness of test element up to 70 cm.
  - Temperature range -20 – 80 °C.
  - Measurement speed: ~ 1 day/measurement.
  
- **Big Guarded Hot Box** [8] (see *Figure 5*):
  - Very large full-scale vertical construction element.
  - Square element with dimensions 4 x 4 m.
  - Thickness of test element up to 1 m.
  - Temperature range -20 – 80 °C.
  - Measurement speed: ~ 2 day/measurement.

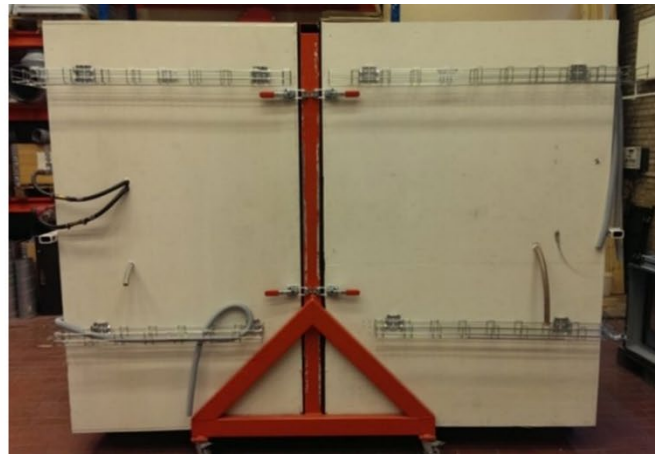

**Figure 4:** The Guarded Hot Box setup at Aalborg University, Department of the Built Environment.



**Figure 5:** The Big Guarded Hot Box setup at Aalborg University, Department of the Built Environment [8].

### 3.2. Specific Heat Capacity

Very small samples can be characterized with a Differential Scanning Calorimetry (DSC) Apparatus. The specific heat capacity of small samples can be measured with the Laser Flash Analysis Apparatus LFA 447 [5]. It is also possible to measure the local specific heat capacity of a larger sample with the scanning mode of the Laser Flash Analysis Apparatus LFA 447. The specific heat capacity of medium-size samples can be measured with a modified Guarded Hot Plate apparatus operating in dynamic mode.

- **Laser Flash Analysis Apparatus LFA 447 [5]** (see *Figure 6*):
  - Thin sample of uniform thickness with smooth surfaces (no fibers or large pores structures).
  - Powder, liquid, slurry, layered material, graded material, anisotropic material.
  - Temperature range 10 – 300 °C.
  - Round sample of diameter 6 mm\*; 8 mm\*; 10 mm\*, 12.7 mm\*, 25.4 mm\*. Thickness 0.5 – 3 mm. \*can be diameter down to 1.2 mm less than prescribed diameter.
  - Scanning mode local measurement of large sample: round diameter 40 mm; square 50 x 50 mm. Resolution of 0.1 mm.
  - Measurement uncertainty: 5 %.
  - Measurement speed: ~ 3 min/measurement.



**Figure 6:** Laser Flash Analysis Apparatus LFA 447 (Netzsch Gerätebau GmbH) [5].

- **Guarded Hot Plate Apparatus EP500** – modified dynamic version [4][6] (see *Figure 7*):
  - Cubical sample of uniform thickness with flat surfaces (compression of sample is controlled).
  - Temperature range 10 – 40 °C.
  - Compression pressure range 0.05 - 2.5 kN/m<sup>2</sup> (5000 - 25000 Pa).
  - Sample dimension : 15 x 15 cm for conductive material, 50 x 50 cm for insulating material.
  - Sample thickness range 1 – 12 cm.



**Figure 7:** The Guarded Hot Plate Apparatus EP500 from Lambda-Messtechnik GmbH Dresden [6].

- **Differential Scanning Calorimetry (DSC) Apparatus Netzsch Jupiter STA 449 F5 and Jupiter STA 449 F3 (see Figure 8):**
  - Temperature range 100 – 900 °C (F5); -150 – 600 °C (F3 with liquid nitrogen).
  - Sample dimension: a few grams.
  - Sample conditioning: Compressed air or nitrogen gas (F5); helium or nitrogen gas (F3); sample placed in aluminum crucible.
  - Measurement uncertainty: 2 %.
  - Measurement speed: 6h/sample (3 scans: empty crucible, standard sapphire, test sample; with autosampler).



**Figure 8:** Differential Scanning Calorimetry Apparatus Jupiter STA 449 F3 (Netzsch Gerätebau GmbH) [5].



### 3.3. Thermal Diffusivity

The thermal diffusivity of small samples can be measured with the Laser Flash Analysis Apparatus LFA 447 [5][7]. It is also possible to measure the local specific heat capacity of a larger sample with the scanning mode.

- **Laser Flash Analysis Apparatus LFA 447 [6][8] (see Figure 9):**
  - Thin sample of uniform thickness with smooth surfaces (no fibers or large pores structures).
  - Powder, liquid, slurry, layered material, graded material, anisotropic material.
  - Thermal diffusivity range  $0.01 - 1000 \text{ mm}^2/\text{sec}$ .
  - Temperature range  $10 - 300 \text{ }^\circ\text{C}$ .
  - Round sample of diameter 6 mm\*; 8 mm\*; 10 mm\*, 12.7 mm\*, 25.4 mm\*. Thickness 0.5 – 3 mm. \*can be diameter down to 1.2 mm less than prescribed diameter.
  - Scanning mode local measurement of large sample: round diameter 40 mm; square 50 x 50 mm. Resolution of 0.1 mm.
  - Measurement uncertainty: 3 %.
  - Measurement speed:  $\sim 3 \text{ min/measurement}$ .



**Figure 9:** Laser Flash Analysis Apparatus LFA 447 (Netzsch Gerätebau GmbH) [6].

## 4. Air transport properties

### 4.1. Effective Air Permeability

The effective air permeability of medium-size samples of porous materials can be measured at room temperature with an air permeameter [10].

- **Air permeameter** [10] (see *Figure 10*):
  - Medium-size sample of porous materials uniform thickness.
  - Cubical samples: 50 x 50 cm (squared section); thickness 1 – 20 cm.
  - Room temperature and relative humidity (possible to condition sample in specific temperature and relative humidity environment inside climatic room).
  - Measurement uncertainty: 2% - 20% ( $3\sigma$  confidence interval).
  - Measurement speed: 1 hour/test sample.





**Figure 10:** Air permeameter setup [10].



## 4.2. Gas Diffusion Coefficient

The gas diffusion coefficient characterizes how permeable to gas is a porous material. It can be measured with the Oxygen Diffusion Apparatus ODA 20, an instrument that has developed at Aalborg University [14].

- **ODA 20** (see Figure 11):
  - Small-size cylindrical test sample: diameter 53 mm, length 50 mm.
  - Measurement speed: ~ 1-3 hour/measurement (10 samples at a time in parallel setups).
  - Room temperature and room relative humidity (possibility to control it with climatic room).

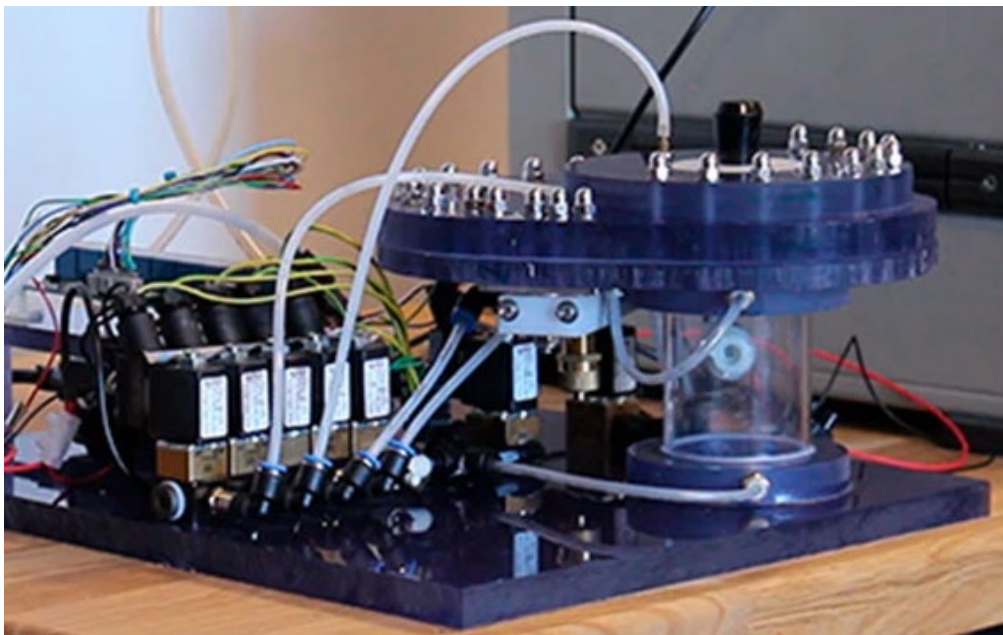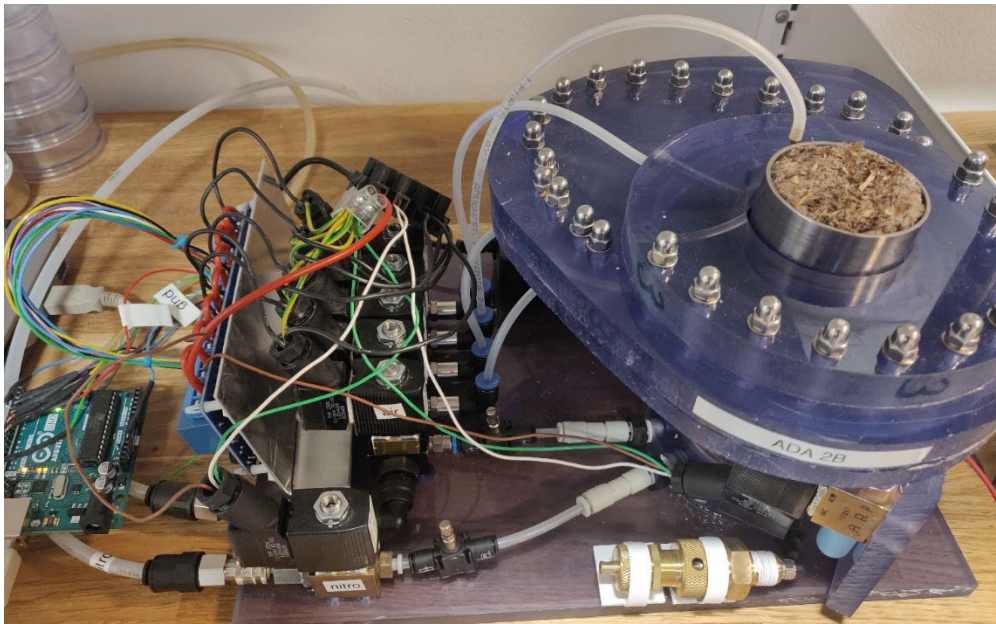

**Figure 11:** The oxygen diffusion apparatus ODA 20 for the measurement of the gas diffusion coefficient in porous materials [14].

## 5. Moisture Transport and Dynamics Properties

### 5.1. Hygrothermal Properties: Water Vapor Sorption and Desorption Capacity

The moisture transfer, retention and release capacity of materials can be determined by measuring water vapor sorption and desorption isotherms. This can be done by the AquaLab VSA [13] with both the static and the dynamic isotherms methods: Dynamic Vapour Sorption (DVS) and Dynamic Dew Point Isotherm (DDI). The VSA Apparatus is much faster and simpler than other conventional methods.

- **AquaLab VSA** apparatus [13] (see *Figure 12*):
  - Small-size test sample: mass range 500 – 5000 mg.
  - Sample holder volume 10 cm<sup>3</sup>.
  - Dynamic Vapour Sorption (DVS) and Dynamic Dew Point Isotherm (DDI).
  - Relative humidity range 3 – 95 %.
  - Temperature range 15 – 60 °C.
  - Measurement accuracy of relative humidity 0.5 %.
  - Temperature stability  $\pm 0.1$  °C.
  - Mass resolution 0.5 mg.
  - Measurement speed:  $\sim 2$  days/full isotherm.





**Figure 12:** AquaLab VSA (METER Group) [13].



## 5.2. Gas Diffusion Coefficient

The gas diffusion coefficient characterises how permeable to gas is a porous material. It can be measured with the Oxygen Diffusion Apparatus ODA 20, an instrument that was developed at Aalborg University [14].

- **ODA 20** (see Figure 13):
  - Small-size cylindrical test sample: diameter 53 mm, length 50 mm.
  - Measurement speed: ~ 1-3 hour/measurement (10 samples at a time in parallel setups).
  - Room temperature and room relative humidity (possibility to control it with climatic room).

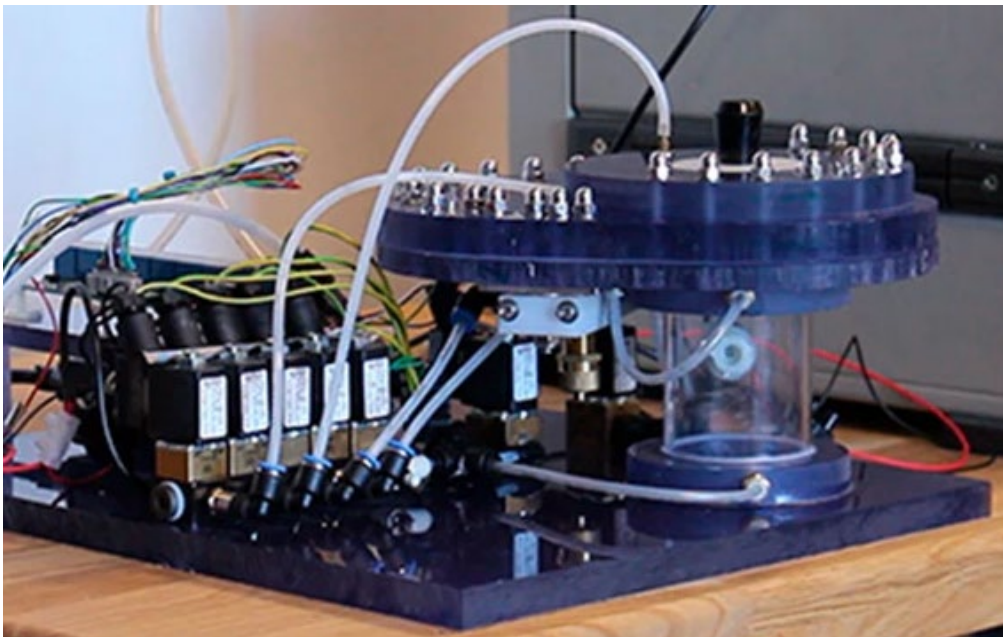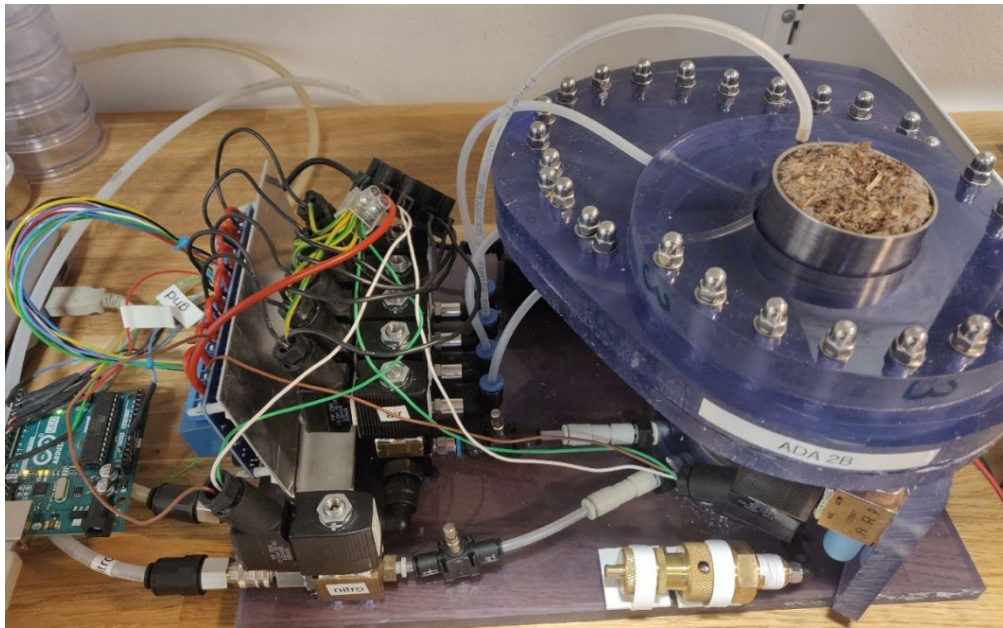

**Figure 13:** The oxygen diffusion apparatus ODA 20 for the measurement of the gas diffusion coefficient in porous materials [14].

### 5.3. Water Vapor Permeability

The water vapor permeability characterizes how permeable to water vapor is a porous material. It can be measured with the Wet/Dry Cup method with the help of a climatic chamber for temperature and relative humidity control. Dedicated 3D-printed sample holders have been designed at Aalborg University to perform the Wet/Dry Cup method accurately.

- **Wet/Dry Cup method** [according to EN ISO 12572 with silica gel as drying agent](see *Figure 14*):
  - Small-size cylindrical test sample: diameter 49 mm, length 51 mm (sides sealed with rubber sealant).
  - Measurement speed: ~ 2-10 weeks/measurement.
  - Temperature range 10 °C - 95 °C (with climatic chamber VCL 7010 – Vötsch Industrietechnik [11]).
  - Relative humidity range 10 - 98 % (with climatic chamber VCL 7010 – Vötsch Industrietechnik [11]).



**Figure 14:** 3D-printed sample holder with bio-based material inside it for Wet/Dry Cup method (left); several Wet/Dry Cup method tests running in the climatic chamber VCL 7010 – Vötsch Industrietechnik [11] (right).

### 5.3. Humidity Content

The humidity content of a moist material is measured by continuously monitoring the mass loss of the test sample (with a precision scale) when it is drying in an oven (see *Figure 15*).

- Oven temperature range room temperature - 300 °C.
- Interior volume 115 L.
- Measurement method speed: ~ 1 week.



**Figure 15:** Drying oven FP 115 (BINDER GmbH) [12].

## References

- [1] Building Material Characterization Laboratory of Aalborg University, Department of the Built Environment, Aalborg, Denmark.  
<https://www.en.build.aau.dk/lab/building-material-characterization>
- [2] Mettler Toledo, Laboratory weighing applications, Density measurement.  
[https://www.mt.com/ch/en/home/applications/Laboratory\\_weighing/density-measurement.html](https://www.mt.com/ch/en/home/applications/Laboratory_weighing/density-measurement.html)
- [3] Sartorius Lab Instruments GmbH & Co, Laboratory weight balances.  
<https://www.sartorius.com/en/products/weighing/laboratory-balances>
- [4] Hicham Johra. Description of the Guarded Hot Plate Method for thermal conductivity measurement with the EP500. DCE Lecture Notes No. 75. Department of Civil Engineering, Aalborg University, 2019.  
[https://vbn.aau.dk/ws/portalfiles/portal/317020205/Description\\_of\\_the\\_Guarded\\_Hot\\_Plate\\_Method\\_for\\_Thermal\\_Conductivity\\_Measurement\\_with\\_the\\_EP500.pdf](https://vbn.aau.dk/ws/portalfiles/portal/317020205/Description_of_the_Guarded_Hot_Plate_Method_for_Thermal_Conductivity_Measurement_with_the_EP500.pdf)
- [5] Netzsch Gerätebau GmbH. Product brochure STA 449 F5 Jupiter: <https://analyzing-testing.netzsch.com/en/products/simultaneous-thermogravimetry-differential-scanning-calorimetry-sta-tg-dsc/sta-449-f5-jupiter>
- [6] Netzsch Gerätebau GmbH. Operating Instructions Nano-Flash-Apparatus LFA 447, 2001.
- [7] <http://www.lambda-messtechnik.de/en.html>
- [8] Hicham Johra. Description of the laser flash analysis method for thermal diffusivity measurement with the LFA 447. DCE Lecture Notes No. 73. Department of Civil Engineering, Aalborg University, 2019.  
[https://vbn.aau.dk/ws/portalfiles/portal/312969074/Description\\_of\\_the\\_Laser\\_Flash\\_Analysis\\_Method\\_for\\_Thermal\\_Diffusivity\\_Measurement\\_with\\_the\\_LFA\\_447.pdf](https://vbn.aau.dk/ws/portalfiles/portal/312969074/Description_of_the_Laser_Flash_Analysis_Method_for_Thermal_Diffusivity_Measurement_with_the_LFA_447.pdf)
- [9] Martin Veit, Hicham Johra. Experimental Investigations of a Full-Scale Wall Element in a Large Guarded Hot Box Setup: Methodology Description. Technical Reports No. 304. Department of the Built Environment, Aalborg University, 2022. <https://doi.org/10.54337/aau488363266>
- [10] Hicham Johra. Air permeameter for porous building materials: Aalborg University prototype 2023. Lecture Notes No. 84. Department of the Built Environment, Aalborg University, 2023.  
<https://doi.org/10.54337/aau545266824>.
- [11] Vötsch 2009 VTL and VCL for Temperature and Climatic Tests URL.  
[https://www.citrotek.dk/images/2009\\_laborhelfer\\_E\\_06.pdf](https://www.citrotek.dk/images/2009_laborhelfer_E_06.pdf).
- [12] BINDER GmbH, Drying oven chamber FP 115.  
<https://www.binder-world.com/en/products/drying-and-heating-chambers/series-fp-classicline/fp-115>
- [13] Vapor Sorption Analyzer AquaLab.  
<https://www.metergroup.com/food/products/vsa/>
- [14] K.M. Frandsen, Y.I. Antonov, H. Johra, P. Møldrup, R.L. Jensen (2021). Experimental investigation of water vapor diffusivity in bio-based building materials by a novel measurement method. Proceedings of the Resilient Materials 4 Life (RM4L) 2020 International Conference. Cambridge, United Kingdom, 20-23 September 2021.  
<https://orca.cardiff.ac.uk/id/eprint/145287/1/RM4L2020%20Conference%20Proceedings%20-%20Online%20Version.pdf>.

### **Recent publications in the DCE Lecture Note Series**

Hicham Johra. Measurement Capabilities and Equipment at the Building Material Characterization Laboratory of Aalborg University (2020). DCE Latest News No. 59. Department of Civil Engineering, Aalborg University, 2019.

