

Determination of organic micro-pollutants such as personal care products, plasticizers and flame retardants in sludge

Chen, Xijuan; Bester, Kai

Published in:
Analytical and Bioanalytical Chemistry

DOI (link to publication from Publisher):
[10.1007/s00216-009-3138-5](https://doi.org/10.1007/s00216-009-3138-5)

Publication date:
2009

Document Version
Publisher's PDF, also known as Version of record

[Link to publication from Aalborg University](#)

Citation for published version (APA):
Chen, X., & Bester, K. (2009). Determination of organic micro-pollutants such as personal care products, plasticizers and flame retardants in sludge. *Analytical and Bioanalytical Chemistry*, 395(6), 1877-1884.
<https://doi.org/10.1007/s00216-009-3138-5>

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal -

Take down policy

If you believe that this document breaches copyright please contact us at vbn@aub.aau.dk providing details, and we will remove access to the work immediately and investigate your claim.

Determination of organic micro-pollutants such as personal care products, plasticizers and flame retardants in sludge

Xijuan Chen · Kai Bester

Received: 18 August 2009 / Accepted: 7 September 2009 / Published online: 25 September 2009
© Springer-Verlag 2009

Abstract In this study, a method for the determination of organic micro-pollutants, i.e. personal care products such as synthetic musk fragrances, household bactericides, organophosphate flame retardants and plasticizers, as well as phthalates in sludge, has been developed. This method is based on lyophilisation and accelerated solvent extraction followed by clean-up steps, i.e. solid phase extraction and size exclusion chromatography. The determination is performed by gas chromatography coupled to mass spectrometry. Stable isotope-labelled compounds such as musk xylene (MX D₁₅), tri-*n*-butylphosphate (TnBP D₂₇) and triphenylphosphate (TPP D₁₅) were used as internal standards. Recovery rates were determined to be 36–114% (with typical relative standard deviation of 5% to 23%) for the target compounds. The limit of detection was 3–30 ng g⁻¹, and the limit of quantification was 10–100 ng g⁻¹ dry matter.

Keyword Personal care products · Musk fragrances · Triclosan · Household bactericides · Organophosphates · Phthalates

Electronic supplementary material The online version of this article (doi:10.1007/s00216-009-3138-5) contains supplementary material, which is available to authorized users.

X. Chen · K. Bester (✉)
Department of Biotechnology,
Chemistry and Environmental Engineering, Aalborg University,
Sohngaardsholmsvej 57,
9000 Aalborg, Denmark
e-mail: kb@bio.aau.dk

K. Bester
Institute of Environmental Analytical Chemistry,
University Duisburg-Essen,
Universitätsstr. 15,
45141 Essen, Germany

Introduction

Sewage sludge is produced in waste water treatment while removing compounds causing oxygen demand (BOD₅) from the waste water. Thus sludge contains high concentrations of organic matter, nutrients (nitrogen and phosphorous) and lipophilic organic micro-pollutants from the waste water. Some countries such as the Nordic countries prefer to use the nutrients in agriculture (re-cycling of sludge), while some others (e.g. Switzerland) have decided to incinerate all sludges as they prioritised to destroy all micro-pollutants. The majority of countries do a case by case decision depending on the concentrations of organic micro-pollutants and heavy metals. Thus a sound basis for analysing organic micro-pollutants in sludge is necessary to make sure that only sludge with low contaminations is used for re-cycling in agriculture. Established methods are usually single or group specific such as the methods used to analyse PAHs or PCBs [1, 2]. Often the analytical protocols are similar to those established for sediments with a high load of TOC.

The compounds included in this study were synthetic musk fragrances (musk xylene, musk ketone, HHCB, AHTN, HHCB-lactone), an antimicrobial and its metabolite (triclosan, triclosan-methyl), organophosphate flame retardants and standing for organophosphate-plasticizers (tri-*iso*-butylphosphate (TiBP), tri-*n*-butylphosphate (TnBP), tris-(2-chloroethyl) phosphate (TCEP), tris-(2-chloro-*iso*-propyl) phosphate (TCPP), tris-(dichloro-*iso*-propyl) phosphate (TDCP) and triphenylphosphate (TPP)) and the phthalate (di(2-ethylhexyl) phthalate (DEHP); Table S1). Some of these compounds have been discussed in national as well as developing EU laws on sludge as maker compounds for the re-use of this material [3, 4].

Synthetic musk fragrances are compounds used as low cost fragrances in soaps, perfumes, air fresheners, deter-

gents, fabric softeners and other household cleaning products. There are four synthetic musk fragrances accounting for 95% of the used musk. These are two polycyclic compounds (HHCB and AHTN) as well as the nitro-musks (musk xylene and musk ketone). These compounds have been detected in surface water [5, 6], in waste water [7–9] and in sewage sludge [10–12]. HHCB–lactone is the primary metabolite of HHCB (Table S1). The ratio HHCB versus its metabolite HHCB–lactone has been used to detect transformation processes of this fragrance. During the sewage treatment process, about 10% of HHCB is transformed to HHCB–lactone, which has been reported for balance assessment for polycyclic musk fragrances in a German treatment plant by Bester [8]. Reviews of several analytical strategies for the analysis of musks in sludge have been described by using accelerated solvent extraction (ASE), supercritical fluid extraction, Soxhlet extraction and liquid–liquid extraction, all of them in combination with gas chromatography–mass spectrometry (GC–MS) [13–15].

Triclosan (Table S1) is an antimicrobial agent, which is widely used in personal care products such as toothpaste, soaps, deodorants, cosmetics and skin care lotions as well as other consumer goods. Approximately 1,500 t is produced annually worldwide, and approximately 350 t of those is applied in Europe [16]. Triclosan–methyl (Table S1) is a transformation product of triclosan. These two compounds have been identified in the environment by several investigators [16–21], whereas bioaccumulation and toxicity have been studied by Orvos et al. [22], Coogan et al. [23] and De Lorenzo et al. [24]. Analytical methods for analysing antimicrobials in sludge by using GC–MS and liquid chromatography–MS have been reviewed by Peck [13].

The organophosphates included in this study were chlorinated alkylphosphates such as TCPP, TCEP and TDCP, which are mostly used as flame retardants in polyurethane. Additionally, non-derivatised alkylphosphates such as the two isomers of tri-butylphosphate (*Tn*BP and *Ti*BP) and TPP, which are used as plasticisers, were studied as well. Because of their relatively low cost, organophosphates especially TCPP have become the most widely used class of flame retardants [25]. These compounds are washed off from the equipped items during cleaning; the cleaning water will be discharged to the sewer and thus reach waste water treatment plants, as discussed by Fries and Puttmann [26] as well as by Meyer and Bester [27]. Additionally, these organophosphates have been detected in indoor air as well as in indoor dust by Sanchez et al. [28] and García et al. [29]. Only a few analytical procedures to determine organophosphates in sludge or sediment with high TOC content have been described [30, 31].

DEHP is one of the most widely used plasticizers. It is used mainly for making PVC soft and pliable. This

plasticizer is eluted into waste water by washing and cleaning processes of the respective materials; it is assumed to have ecotoxic (endocrine disrupting) effects to aquatic organisms [32]. Because of the relatively high lipophilicity of this phthalate, sorption is the main process relevant for elimination in sewage treatment plants. Typical concentration of DEHP in sludge was found to be ranging from 10 to 100 $\mu\text{g L}^{-1}$ by Fromme et al. [33]. Extraction methods in combination with GC–MS have been described by Sablayrolles et al. [34] and Aparicio et al. [35].

The main objective of the research presented in this paper was to develop and validate an analytical multi-method to determine different classes of organic micro-pollutants such as personal care products, plasticizers and flame retardants and phthalates in sludge.

Experimental section

Materials

AHTN, triclosan, musk xylene, musk ketone and DEHP were purchased from Ehrenstorfer (Augsburg, Germany) as pure compounds with purities being $\geq 99\%$ according to the supplier. Pure standards of HHCB–lactone as well as HHCB were obtained from International Flavours and Fragrances (IFF, Hilversum, Netherlands). Triclosan–methyl was synthesised from triclosan by methylation with trimethylsulfonium hydroxide solution (Macherey–Nagel, Dueren, Germany) at 40°C [20].

TCPP and TDCP were obtained from Akzo Nobel (Amersfoort, the Netherlands). These compounds were used without further purification. The technical TCPP gives three peaks in the ratio 9:3:1. In this study, only the main (first eluting) isomer was used for determination. *Tn*BP, *Ti*BP, TPP and TCEP were purchased from Sigma-Aldrich (Steinheim, Germany). Ethyl acetate, acetone, cyclohexane and methanol were used in analytical grade (p.a.) quality, while toluene and *n*-hexane were used in residue grade (z.R.) quality. All solvents were purchased from Merck (Darmstadt, Germany).

Internal standards

The internal standard musk xylene D_{15} was used to quantify the musk fragrances musk xylene, musk ketone, HHCB, AHTN, triclosan–methyl and DEHP as it elutes in the same fraction as these compounds, while *Tn*BP D_{27} was used to quantify *Ti*BP, *Tn*BP, TCEP and TCPP, and TPP D_{15} was used in this experiment to quantify triclosan, HHCB–lactone, TDCP and TPP. Musk xylene D_{15} and *Tn*BP D_{27} were obtained from Ehrenstorfer (Augsburg,

Germany); TPP D₁₅ was synthesised from D₆ phenol and phosphoroylchloride. These internal standards were chosen as they give undisturbed signal and also do not undergo any reaction themselves [36].

Analytical method

The sample preparation scheme is shown in Fig. 1: After sampling, the sludge samples were immediately frozen at -27°C overnight. “Dried sludge” such as produced at waste water treatment plants contains about 70% water; thus drying is essential to provide good wettability of the sludge with organic solvents. The frozen sub-samples of 40 g wet weight were then lyophilised overnight at 2 mbar and -46°C using an ALPHA 1-2/LD (Christ, Osterode am

Harz, Germany). The 4–6 g lyophilised sludge samples was blended with about 10 g diatomaceous earth (acid-washed obtained from MP Biomedicals, Solon, OH, USA) and homogenised in a mill (IKA A11 BASIC, Staufen, Germany) to a fine powder. The homogenates were then transferred into a 33-mL stainless steel ASE cell and extracted successively with ethyl acetate (ASE 200, Dionex, Sunnyvale, USA). After adding an aliquot of 500 μL internal standard solution (IS; containing 500 ng D₁₅ musk xylene, 500 ng TPP D₁₅ and 500 ng TnBP D₂₇), the extract was concentrated to 1 mL by a Büchi Synchore multiport concentrator (Büchi, Essen, Germany) at 80°C and 70 mbar.

The resulting extracts were cleaned up with silica solid phase extraction (SPE) cartridges. This step is primarily protecting the next step (size exclusion chromatography (SEC)) from too many particles as well as very polar compounds. It was performed by packing 1 g of silica (silica 60 obtained from Merck, Darmstadt, Germany, pre-dried at 105°C) into a glass column (60 mm long, 12 mm ID) with two PTFE frits on the top and bottom of silica. The silica column was conditioned with 12 mL *n*-hexane before use and eluted with 12 mL ethyl acetate after loading the samples.

The resulting extracts were again concentrated by a Büchi Synchore multiport concentrator and successively injected into an SEC system (GPC-Basix, purchased from LC-Tech, Dorfen, Germany) equipped with a glass column ID: 2.5 cm, length 30 cm, packed with 50 g SX-3 (Bio-Rad, Hercules, CA, USA). The mobile phase was cyclohexane and ethyl acetate (1:1, *V/V*) and the flow rate was 5.0 mL min^{-1} . The solvent eluting in the first 19.30 min (97.5 mL) containing macro-molecules was drained to waste, while the fraction 19.30–30.00 min (52.5 mL) containing the analytes was collected [37]. The samples were finally transferred into toluene by adding 10 mL toluene and condensing to 1 mL. Thus, macro-molecules were separated as they are eluted in the first fraction, while sulphur, etc. are separated from the target compounds as they are eluted after the analyte fraction.

The resulting extracts were then fractionated for polarity on silica 60 using 12 mL 5% methyl-*tert*-butylether in *n*-hexane (first fraction) and 12 mL ethyl acetate (second fraction) successively as eluents. The musks, triclosan-methyl and DEHP were eluted in the first fraction, while TiBP, TnBP, TCEP, TCPP, TDCP and TPP as well as triclosan and HHCB-lactone were eluted in the second fraction according to their polarity. These fractions were transferred into toluene as described above and finally analysed by GC-MS detection.

The GC-MS system was a DSQ purchased from Thermo, Waltham, USA. The GC was equipped with a programmable temperature vapouriser (PTV) injector. The

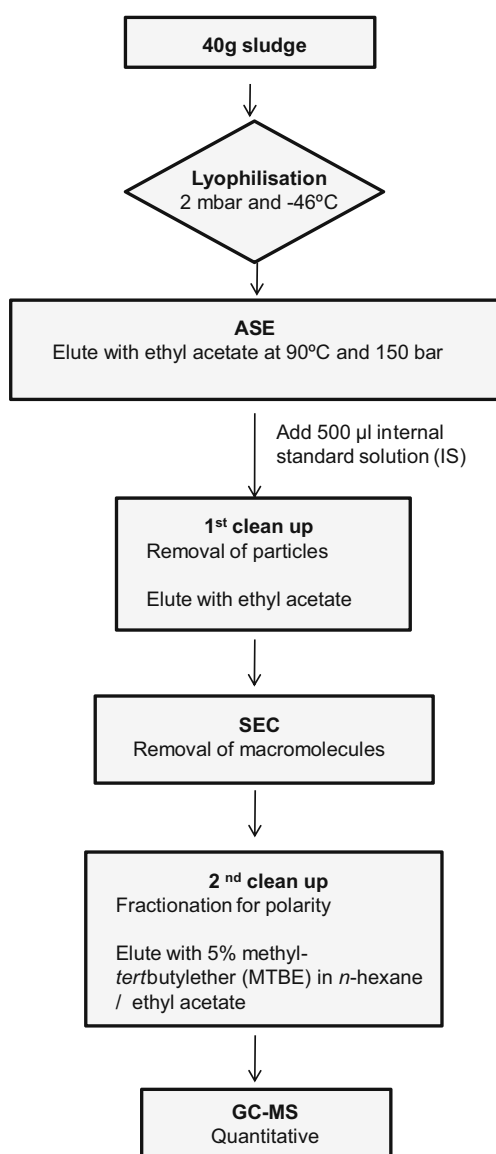


Fig. 1 Sample preparation scheme

PTV (1 μL injection volume) was operated in PTV splitless mode. The injection temperature of 115°C was held for 3 s; it was successively ramped with 12 to $280^{\circ}\text{C s}^{-1}$ for the transfer of the analytes into the column. This temperature was held for 1.3 min. The injector was then ramped with 1 to $300^{\circ}\text{C s}^{-1}$ (open split), which was held for 7 min as a cleaning phase.

The GC separation was performed with a DB-5MS column (J&W Scientific), L was 15 m, ID was 0.25 mm, and film thickness was $0.25\text{ }\mu\text{m}$. The oven temperature programme started at 100°C (hold, 1 min) and was then ramped with 30 to $130^{\circ}\text{C min}^{-1}$ and successively with 8 to $220^{\circ}\text{C min}^{-1}$. Finally, the baking temperature was reached by ramping the oven with 30 to $280^{\circ}\text{C min}^{-1}$, which was held for 7 min.

The transfer line was held at 250°C , which is sufficient to transfer all compounds from the GC into the MS as the vacuum builds up in the transfer line. The ion source was operated at 230°C . Helium (4.0) was used as carrier gas with a flow rate of 1.3 mL min^{-1} . All compounds were detected by means of their mass spectral data and retention times as shown in Table 1.

Calibrations were performed as a multi-step internal standard calibration. A stock solution was produced by dissolving 20 mg of the target compounds into 100 mL acetone. This stock solution was stored at 4°C in the dark. The weight of this flask was controlled before and after each operation. Calibration standards (3, 10, 30, 100, 300, 1,000, 3,000 and $10,000\text{ ng mL}^{-1}$ in toluene) were made by serial dilution of the stock solution. The calibration standards contained the internal standards with a concentration of 100 ng mL^{-1} . The calibration curve was calculated by using a weighted ($1/X$) linear regression.

Results and discussions

Extracting organic compounds from sludge is optimised between extracting as much as possible of the target compound and as little as possible of the organic matter of the sludge, as the latter will be corrupting the GC or either one of the following steps.

Three experiments were performed to determine the optimal conditions for the accelerated solvent extraction in the method development and method validation after it had been decided to focus on ethyl acetate as an extractant:

1. A temperature optimisation, which was compared to total and destructive extractions
2. Validation from an artificial blank material to determine potential concentration dependency of the recovery rate as well as blank problems
3. Validation from a spiked sludge to determine recovery rates by different means as well as gain insight on realistic precision

Optimisation of extraction temperature

Temperature is the most important parameter used in ASE extraction. ASE operates at temperatures above the normal boiling point of most solvents, using pressure to keep the solvents in the liquid phase during the extraction process. As the temperature is increased, the viscosity of the solvent is reduced, thereby increasing its ability to wet the matrix and solubilise the target analytes. However thermal degradation of the solvent or the sample might occur at higher temperatures [38, 39]. In this study a temperature range from 50 to 150°C was tested for the optimisation of

Table 1 Retention times and selected mass fragments for the determination of the respective compounds using a DB-5 column

Compound	RT (min)	Quantifier mass (amu)	Verifier mass (amu)
OTNE	5.96	191	219
Musk xylene	8.12	282	297
Musk ketone	9.50	279	294
HHCB	8.03	243	258
AHTN	8.14	243	258
HHCB-lactone	11.73	257	272
Triclosan	11.07	288	290
Triclosan-methyl	11.30	302	304
TiBP	4.37	155	211
TnBP	5.80	155	211
TCEP	7.19	249	251
TCPP	7.46	277	279
TDCP	13.35	379	381
TPP	13.88	325	326
DEHP	14.60	149	167

extraction. For the extraction of organic micro-pollutants, one sub-sample of homogenised dried sludge was extracted by ASE with temperatures of 50, 70, 90, 110, 130 and 150°C, each followed by first clean up, SEC and the second clean up as described above. In the end the samples were measured by GC–MS. The highest concentration of HHCB, AHTN, triclosan and HHCB–lactone was found from the 70 and 90°C extractions, which is shown in Fig. 2. The increased concentration of HHCB–lactone found at 130°C was interpreted as result of an oxidation of HHCB under these conditions. Therefore, 90°C was selected as the extraction temperature because of the better extraction efficiency proved here and suggested references [38, 39]. As a control, total extractions with acetone and acidified methanol at 150°C were performed. These did not give higher concentrations than those with ethyl acetate at 90°C and 150 bar.

Method validation from artificial blank material (manure/soil) recovery rates and working range

These experiments were performed to determine whether the recovery rate was dependent on the concentration or not. The working range was considered to range from the lowest to the highest concentrations for which the same recovery rates were obtained. A blank material, which contains similar TOC and ammonia content as sludge but no analytes, was produced by mixing manure from organic farming with soil (1:1). Various concentrations of the standard were spiked into the dried homogenized material. The spiked sub-samples were transferred into ASE cells, which were extracted with the method described above. Table 2 shows the recovery rate and its working range determined from the spiked artificial blank material. Figure S1 shows the recovery rate of triclosan as the function of concentration. The recovery rates for all compounds are independent on the concentrations (Table 2). It was also demonstrated that no other peaks (e.g. from decomposition/

pyrolysis) of biogenic material that could be mistaken for the analytes occurred from such matrices.

Method validation from spiked sludge samples (LOQ)

These recovery experiments were carried out by providing six homogeneous sub-samples from one sludge sample and each was spiked with 125 µl of the stock solution (200 µg mL⁻¹). Two other sub-samples were left unspiked as comparison. They were lyophilised and then extracted at 90°C and 150 bar. The following sample preparation, extraction and clean up were identical to the procedures described above. For this study, dewatered digested sludge of an urban waste water treatment plant with 450,000 population equivalents, operating BOD, nitrogen and phosphorous removal was used. The sludge had a water content of 90% before lyophilisation. The mineral content of the total solid content was 33%. The concentrations of the target compounds in this sludge before and after spiking are shown in Table 3. Figure 3 shows the chromatographic characterisation of TCPP in one unspiked sludge sample (18,400 ng g⁻¹).

Since the standard deviation from this six spiked samples was low and no outlier was identified, all results were averaged. The mean recovery rates were 36–114%, and the relative standard deviations were 5–23% (Table 3), depending on the respective compounds. The lower recovery rates of musk xylene and musk ketone were possibly due to the occurrence of biotransformation of the nitro-musks during the sample preparation process [40, 41]. The limit of detection was taken as signal-to-noise ratio 3:1, and the limit of quantification (LOQ) was defined as signal-to-noise ratio 10:1, which was calculated by the Xcalibur software (Thermo, Waltham, USA) for the respective SIM chromatograms of the standard calibration (Table 3). The thus obtained LOQs are in the same range as the lower end of the working range (see above, Table 2). Comparable results were obtained by Bester [30] who used a similar procedure

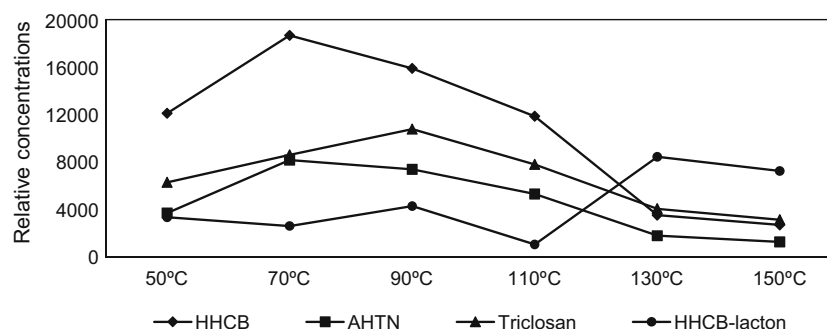


Fig. 2 Relative concentrations of HHCB, AHTN, HHCB–lactone and triclosan obtained by ASE extractions of sludge homogenates at different temperatures

Table 2 Recovery rate and working range determined by the artificial blank material

Compound	Working range (ngg ⁻¹)	RR (%)	RSD (%)
OTNE	30–10,000	73	26
HHCB	300–10,000	87	13
Triclosan	30–10,000	88	9
TiBP	30–10,000	77	6
TCEP	10–10,000	70	11

but utilised a Soxhlet extraction to determine polycyclic musk fragrances and TCPF in waste water treatment plant.

Stereoisomer separation

Stereoisomer-specific determination often gives in-depth insights into ongoing processes; however, this analytical technique is more vulnerable to matrix than conventional analysis, as the respective columns have lower temperature limits. Thus, stereoisomer-specific determination requires better sample clean ups. In this study, it was tested whether the developed sample clean up is suitable also for stereoisomer determination. The gained extracts were used for stereoisomer separation of OTNE. OTNE has two chiral

centres; thus enantiomers and diastereomers may occur. The synthesis of this compound is not stereoselective; thus both kinds of stereoisomers are expected in the product [42].


Stereoisomer separation was performed on a heptakis-(2,3-di-*O*-methyl-6-*O*-*t*-butyldimethyl-silyl)- β -cyclodextrin (Hydrodex 6-TBDMS) column (Macherey-Nagel, Düren, Germany). This column is able to separate enantiomers as well as diastereomers of compounds such as polycyclic musks [15], but for OTNE only two major peaks were observed (Fig. 4). Thorough temperature programme and gas flow optimisation were performed and resulted in a temperature programme of 90 °C [1 min] \rightarrow 10 °C min⁻¹ \rightarrow 115 °C [70 min] \rightarrow 10 °C min⁻¹ \rightarrow 200 °C [30 min] at a constant flow of 1.2 mL min⁻¹ helium gave the best separation from the production impurities. However, only two main stereoisomers could be separated. It is thus currently unknown whether the achieved separation separates the enantiomers or diastereomers of OTNE. However, in this study, it could be demonstrated that the extracts were clean enough to give reliable stereoseparation. A multitude of standards and sludge samples were analysed in one sequence with no change of chromatographic performance. Thus this multi-method is capable to perform sample clean up for stereoseparations as well as conventional analysis.

Table 3 Typical concentration of compounds in sludge samples, mean recovery, relative standard deviation (RSD), limit of detection (LOD) and limit of quantification (LOQ)

Compound	Concentration in unspiked sludge (ngg ⁻¹)	Calculated concentration in spiked sludge (ngg ⁻¹)	Determined concentration (ngg ⁻¹)	Mean recovery rate (%)	RSD (%)	LOD (ngg ⁻¹)	LOQ (ngg ⁻¹)
OTNE	3,000	10,927	6,513	60	6	10	30
MX	80	9,200	4,300	47	19	10	30
MK	40	7,600	2,700	36	23	3	10
HHCB	11,800	20,300	15,700	77	6	3	10
AHTN	1,600	8,900	6,100	69	5	3	10
HHCB-lactone	800	7,900	5,200	66	10	3	10
Triclosan	4,400	11,700	15,600	114	12	30	100
Triclosan-Me	70	7,300	4,000	55	10	3	10
TiBP	100	8,100	6,200	77	10	10	30
TnBP	90	7,700	4,900	64	8	10	30
TCEP	70	11,900	7,000	59	9	10	30
TCPF	18,400	28,000	27,000	96	8	30	100
TDCP	90	8,500	4,400	52	8	10	30
TPP	400	7,600	4,300	57	5	3	10
DEHP	8,700	17,200	15,000	87	21	3	10

The LOD was taken as signal-to noise ratio 3:1, and LOQ was defined as signal-to-noise ratio 10:1, which was calculated by the Xcalibur software (Thermo, Waltham, USA) for the respective SIM chromatograms of the standard calibration. Mean recovery rates were calculated by the ratio of determined concentration and calculated concentration in spiked sludge

Fig. 3 Chromatographic characterisation of the organophosphate flame retardant TCP. The third isomer was not detected as the respective SIM function was aborted before elution of this compound

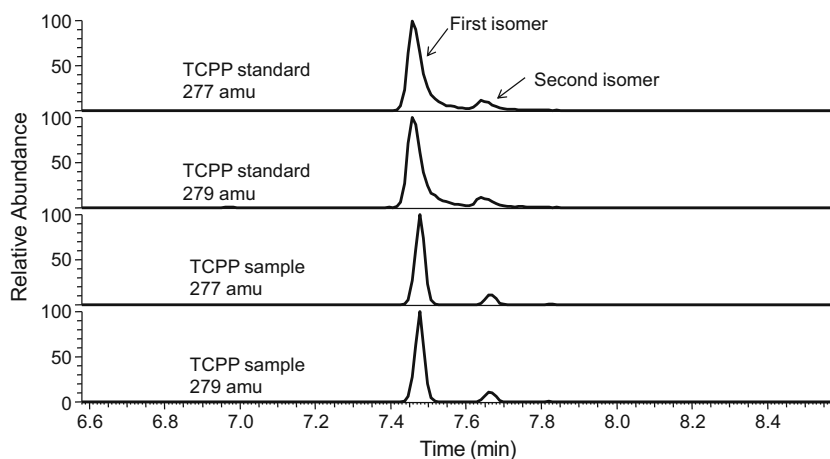

Conclusion

A precise multi-method has been developed to analyse musk fragrances, bactericides as well as organophosphates and flame retardants and phthalate by using lyophilisation, ASE in combination with the clean-up steps of SPE, SEC and the detection of GC-MS. The recovery rates obtained from two different recovery experiments performed by two different operators were comparable. In diverse projects, this method has been used to analyse several hundred sludge samples

especially in degradation and process studies, for which precision as well as stability of the system were crucial. Though the DSQ-MS needs regular cleaning of the curved prefilter quadrupole after injecting about 100 extracts in duplicate plus calibration standards, the method performed well in routine operations. It is a multi-method that in lots of cases is open to including new analytes. Also the extracts were clean enough to perform stereoseparation. Thus a method was validated, which can be the backbone of future research on organic micro-pollutants in sludge.

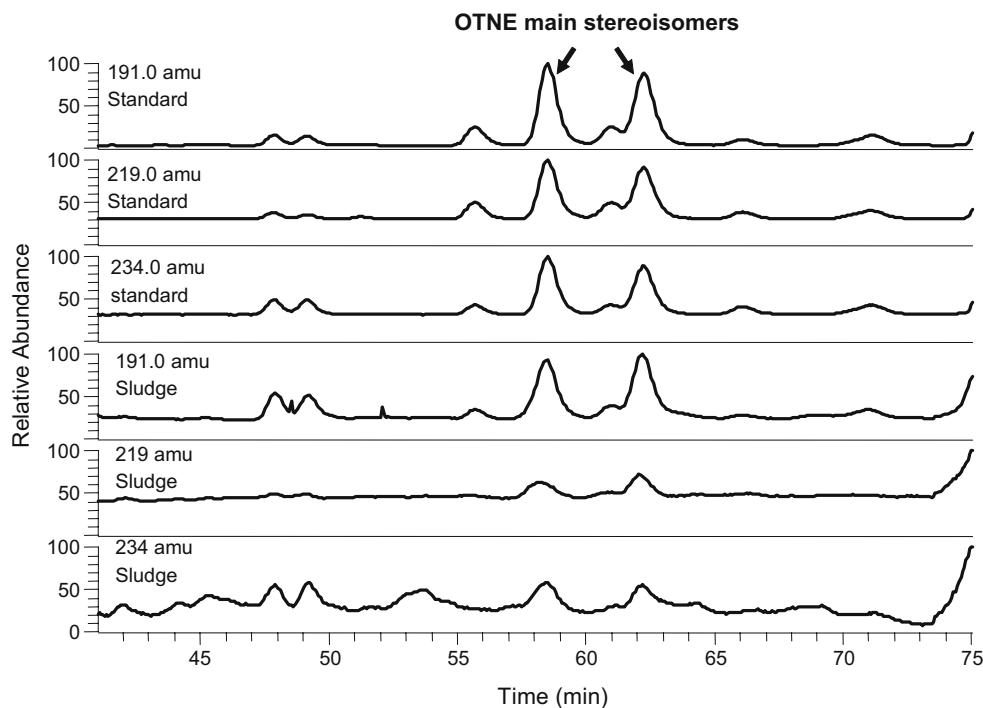


Fig. 4 Separation of stereoisomers of OTNE on a heptakis-(2,3-di-O-methyl-6-O-*t*-butyldimethyl-silyl)- β -cyclodextrin (Hydrodex 6-TBDMS[®]) column. The main stereoisomers were detected at 58.50

and 62.27 min. Temperature programme: 90 °C [1 min] \rightarrow 10 °C min⁻¹ \rightarrow 115 °C [70 min] \rightarrow 10 °C min⁻¹ \rightarrow 200 °C [30 min] at a constant flow 1.2 mL min⁻¹

Acknowledgements The authors acknowledge the support of the Environmental Protection Agency of Northrhine Westphalia through the project “BASPIK”, of the Ministry for Economics through the ProInno/AIF project “Abbau von organischen Schadstoffen im Rahmen der Klärschlammvererdung” and xenobiotic groups of University of Duisburg-Essen as well as the skilled technical laboratory help of Jennifer Hardes for cooperation. Additionally the authors are indebted to the co-operating waste water treatment plant for the possibility to sample their sludge for method development. The authors also acknowledge the support from the project “In situ characterization of microbial degraders of triclosan and methyl-triclosan from wastewater treatment plants” from the Danish research council FTP.

References

- Riley CE (2001) *Waste Manage* 21:465–470
- Sánchez-Brunete C, Miguel E, Tadeo JL (2007) *J Chromatogr A* 1148:219–227
- Pawelczyk A (2005) ISAH. Warsaw, Poland
- Vogel I, Bannick CG, Böken H (2004) Soil and compost ecology. León, Spain
- Peck AM, Hornbuckle KC (2004) *Environ Sci Technol* 38:367–372
- Peck AM, Linebaugh EK, Hornbuckle KC (2006) *Environ Sci Technol* 40:5629–5635
- Garicano EA, Borkent I, Hermens JM, Vaes WJ (2003) *Environ Sci Technol* 37:3111–3116
- Bester K (2004) *Chemosphere* 57:863–870
- Bester K (2005) *J Environ Monit* 7:43–51
- Herren D, Berset JD (2000) *Chemosphere* 40:565–574
- Berset JD, Bigler P, Herren D (2000) *Anal Chem* 72:2124–2131
- Kupper T, Berset JD, Etter-Holzer R, Furrer R, Tarradellas J (2004) *Chemosphere* 54:1111–1120
- Peck AM (2006) *Anal Bioanal Chem* 386:907–939
- Chen X, Pauly U, Rehfus S, Bester K (2009) *Chemosphere* 76:1094–1101
- Bester K (2009) *J Chromatogr A* 1216:470–480
- Singer H, Müller S, Tixier C, Pillonel L (2002) *Environ Sci Technol* 36:4998–5004
- Lopez-Avila V, Hites RA (1980) *Environ Sci Technol* 14:1382–1390
- Paxeus N (1996) *Water Res* 30:1115–1122
- Lindström A, Buerge IJ, Poiger T, Bergqvist PA, Müller MD, Buser HR (2002) *Environ Sci Technol* 36:2322–2329
- Bester K (2003) *Water Res* 37:3891–3896
- Bester K (2005) *Arch Environ Contam Toxicol* 49:9–17
- Orvos DR, Versteeg DJ, Inauen J, Capdevielle M, Rothenstein A (2002) *Environ Toxicol Chem* 21:1338–1349
- Coogan MA, Edziye RE, La Point TW, Venables BJ (2007) *Chemosphere* 67:1911–1918
- DeLorenzo ME, Keller JM, Arthur CD, Finnegan MC, Harper HE, Winder VL, Zdankiewicz DL (2007) *Environ Toxicol* 23:224–232
- IAL Consultants (1999) IAL market report. The European Flame Retardant Chemical Industry 1998. IAL Consultants, London
- Fries E, Puttmann W (2001) *J Environ Monit* 3:621–626
- Meyer J, Bester K (2004) *J Environ Monit* 6:599–605
- Sanchez C, Ericsson M, Carlsson H, Colmsjö A (2003) *J Chromatogr A* 993:103–110
- García M, Rodríguez I, Cela R (2007) *Anal Chim Acta* 590:17–25
- Bester K (2005) *J Environ Monit* 7:509–513
- You J, Lydy MJ (2004) *Arch Environ Contam Toxicol* 47:148–153
- Roh JY, Jung IH, Lee JY, Choi JH (2007) *Toxicology* 237:126–133
- Fromme H, Kuchler T, Otto T, Pilz K, Müller J, Wenzel A (2002) *Water Res* 36:1429–1438
- Sablayrolles C, Montréjaud-Vignoles M, Benanou D, Patria L, Treilhou M (2005) *J Chromatogr A* 1072:233–242
- Aparicio I, Santos JL, Alonso E (2007) *Anal Chim Acta* 584:455–461
- Andresen J, Bester K (2006) *Water Res* 40:621–629
- Bester K, Hühnerfuss H (1997) *Fresenius' J Anal Chem* 358:630–634
- Richter BE, Jones BA, Ezzell JL, Porter NL, Avdalovic N, Pohl C (1996) *Anal Chem* 68:1033–1039
- Vandenburg HJ, Clifford AA, Bartle KD, Zhu SA, Carroll J, Newton LD, Garden LM (1998) *Anal Chem* 70:1943–1948
- Gatarmarm R, Hühnerfuss H, Rimkus G, Attar A, Kettrup A (1998) *Chemosphere* 36:2535–2547
- Käfferlein HU, Göen T, Angerer J (1998) *Crit Rev Toxicol* 28:431–476
- Hicken EJ, Corey EJ (2008) *Org Lett* 10:1135–1138