



Aalborg Universitet

AALBORG
UNIVERSITY

Energy expenditure in critically ill patients estimated by population-based equations, indirect calorimetry and CO₂-based indirect calorimetry

Rousing, Mark Lillelund; Hahn-Pedersen, Mie Hviid; Andreassen, Steen; Pielmeier, Ulrike; Preiser, Jean-Charles

Published in:
Annals of Intensive Care

DOI (link to publication from Publisher):
[10.1186/s13613-016-0118-8](https://doi.org/10.1186/s13613-016-0118-8)

Publication date:
2016

Document Version
Publisher's PDF, also known as Version of record

[Link to publication from Aalborg University](#)

Citation for published version (APA):

Rousing, M. L., Hahn-Pedersen, M. H., Andreassen, S., Pielmeier, U., & Preiser, J.-C. (2016). Energy expenditure in critically ill patients estimated by population-based equations, indirect calorimetry and CO₂-based indirect calorimetry. *Annals of Intensive Care*, 6, Article 16. <https://doi.org/10.1186/s13613-016-0118-8>

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal -

Take down policy

If you believe that this document breaches copyright please contact us at vbn@aub.aau.dk providing details, and we will remove access to the work immediately and investigate your claim.

RESEARCH

Open Access



Energy expenditure in critically ill patients estimated by population-based equations, indirect calorimetry and CO_2 -based indirect calorimetry

Mark Lillelund Rousing^{1*}, Mie Hviid Hahn-Pedersen¹, Steen Andreassen¹, Ulrike Pielmeier¹
and Jean-Charles Preiser²

Abstract

Background: Indirect calorimetry (IC) is the reference method for measurement of energy expenditure (EE) in mechanically ventilated critically ill patients. When IC is unavailable, EE can be calculated by predictive equations or by VCO_2 -based calorimetry. This study compares the bias, quality and accuracy of these methods.

Methods: EE was determined by IC over a 30-min period in patients from a mixed medical/postsurgical intensive care unit and compared to seven predictive equations and to VCO_2 -based calorimetry. The bias was described by the mean difference between predicted EE and IC, the quality by the root mean square error (RMSE) of the difference and the accuracy by the number of patients with estimates within 10 % of IC. Errors of VCO_2 -based calorimetry due to choice of respiratory quotient (RQ) were determined by a sensitivity analysis, and errors due to fluctuations in ventilation were explored by a qualitative analysis.

Results: In 18 patients (mean age 61 ± 17 years, five women), EE averaged 2347 kcal/day. All predictive equations were accurate in less than 50 % of the patients with an RMSE ≥ 15 %. VCO_2 -based calorimetry was accurate in 89 % of patients, significantly better than all predictive equations, and remained better for any choice of RQ within published range (0.76–0.89). Errors due to fluctuations in ventilation are about equal in IC and VCO_2 -based calorimetry, and filtering reduced these errors.

Conclusions: This study confirmed the inaccuracy of predictive equations and established VCO_2 -based calorimetry as a more accurate alternative. Both IC and VCO_2 -based calorimetry are sensitive to fluctuations in respiration.

Keywords: Energy expenditure, Metabolic rate, Caloric intake, Nutritional support, Critically ill, Indirect calorimetry, Respiratory quotient, VCO_2

Background

The determination of energy expenditure (EE) can help clinicians to prescribe caloric intake during the late phase of critical illness, particularly in obese, cachectic or burned patients [1]. The reference method to determine

EE is indirect calorimetry (IC) [2], which uses the Weir equation [3] to provide an estimate of EE from measured oxygen consumption (VO_2) and carbon dioxide production (VCO_2). However, the use of IC is limited by the associated costs, necessary training and demand on resources (e.g., time, equipment and staff) [4, 5]. Furthermore, IC measurements may not be feasible because of logistic or technical difficulties, in about 35–40 % of patients even under conditions of a clinical prospective trial [6, 7].

*Correspondence: mlr@hst.aau.dk

¹ Center for Model-based Medical Decision Support (MMDS), Department of Health Science and Technology, Aalborg University, Fredrik Bajers Vej 7E, 9220 Aalborg East, Denmark

Full list of author information is available at the end of the article

Regardless of the nutritional target, relative to EE, for a patient, EE should be accurately determined. The use of EE determined by predictive equations is recommended when IC cannot be used. For instance, the American College of Chest Physicians (ACCP) equation [8] uses body mass (BM) as the only variable describing the patient: $EE(ACCP) = (25-30 \text{ kcal/kg/day} \cdot BM)$. European [9] and Canadian [10] guidelines concur and both recommend a target of 20–25 kcal/kg/day. Other equations also use the patient's height and age and gender (Harris–Benedict [11] and Mifflin St Jeor [12]). The Penn State equations [13, 14] add respiratory minute volume (MV) and body temperature to further describe the state of the patient.

Reviews by Tatucu-Babet et al. [6] and Frankenfield et al. [15] of the extensive body of the literature on predictive equations conclude that they often are inaccurate. Both reviews used a $\pm 10\%$ difference between the predictive equations and IC to assess over- or underestimations of EE. Frankenfield et al. [15] found that the four equations reviewed all had over- and/or underestimations larger than 10 % in at least 18 % of the patients. Tatucu-Babet et al. [6] found that 12 % of the reviewed predictive equations on average over the patient group studied overestimated EE by more than 10 % and up to 66 % in individual patients. Underestimation was even more frequent with 38 % of the equations underestimating EE by more than 10 % and up to 41 % in individual patients. The frequent underestimations were partially compensated for by multiplying the EE estimated by the predictive equations by a stress factor (SF) and most of the studies evaluating the Harris–Benedict equation used a SF, which ranged from 1.13 to 1.6. This large range of SF may partially be due to interpatient differences, but also to systematic variations of SF due to the severity and type (sepsis, trauma/surgery, burns) of insult [16–18] as well as the time elapsed since the insult [16, 17]. The value of SF is therefore cohort specific, depending on both patient mix and other clinical circumstances.

An alternative may be “VCO₂-based calorimetry” where EE is calculated only from VCO₂, routinely measured by capnometers connected to the ventilatory circuit in mechanically ventilated patients [19]. In this paper, we investigate a method to calculate the VCO₂-based EE from a modified Weir equation [3]: $EE(VCO_2) = ((5.5 \text{ min/ml} \cdot RQ^{-1} + 1.76 \text{ min/ml}) \cdot VCO_2 - 26) \text{ kcal/day}$ [20]. In a clinical application of VCO₂-based calorimetry where VO₂ is not measured, the respiratory quotient (RQ) for the individual patient is unknown and a value of RQ for the individual patient must therefore be chosen. This value may be set to the average from a patient cohort [20, 21] or can be individualized by calculating it from the patient's nutrition

[22, 23]. The purpose of this study is to determine the accuracy of VCO₂-based calorimetry using the modified Weir equation stated above compared with the accuracy of commonly used predictive equations for EE, using IC as the reference method. In clinical practice, the VCO₂ measurements are presumably taken using the ventilator's capnometer. The scope of this paper is not the potential discrepancy between VCO₂ measurements from capnometers in metabolic monitors and in ventilators, but only the accuracy of the VCO₂-based calorimetry compared with IC. Possible sources of error in the VCO₂-based calorimetry and IC will be assessed by a qualitative analysis of data, including a sensitivity analysis of the choice of RQ value.

Methods

Patients

An observational trial was conducted at a mixed medical/postsurgical intensive care unit (ICU) at Erasme University Hospital of Brussels, Belgium. No ethics committee approval was necessary as only noninvasive and anonymized data were collected. Eighteen patients 18 years or older were included as soon as possible after ICU admission, if they were intubated and mechanically ventilated. Height, gender, body mass, temperature, diagnosis, mode of ventilation, APACHE 2 score at admission [24], and sedation were recorded. VO₂, VCO₂, end-tidal CO₂ (ET-CO₂), FiO₂, MV and RQ were measured over a 30-min period. The metabolic monitor used was a Compact Airway Module, E-CAiOVX, mounted in a Compact Anesthesia Monitor (GE Healthcare, Little Chalfont, Buckinghamshire, UK), which offers continual VCO₂ and VO₂ measurements [25]. The Compact Airway Module determines VCO₂ and VO₂ within $\pm 10\%$ when FiO₂ < 65 % [26].

EE is determined, using the Weir Eq. (3):

$$EE(IC) = (5.5 \text{ min/ml} \cdot VO_2 + 1.76 \text{ min/ml} \cdot VCO_2 - 1.99 \text{ day/g} \cdot N) \text{ kcal/day} \quad (1)$$

with a standard setting of $N = 13 \text{ g/day}$ [26], as ureic nitrogen was not measured in the study, yielding:

$$EE(IC) = (5.5 \text{ min/ml} \cdot VO_2 + 1.76 \text{ min/ml} \cdot VCO_2 - 26) \text{ kcal/day} \quad (2)$$

In this study, this is used as the reference method, against which other EE estimates are compared.

Equations for estimation of EE

The equation for estimating EE based on VCO₂ was constructed from Eq. 2, with VO₂ substituted by:

$$VO_2 = VCO_2/RQ \quad (3)$$

This gives the modified Weir equation:

$$\text{EE}(\text{VCO}_2) = \left((5.5 \text{ min/ml} \cdot \text{RQ}^{-1} + 1.76 \text{ min/ml}) \cdot \text{VCO}_2 - 26 \right) \text{ kcal/day} \quad (4)$$

VCO_2 measurements used in the $\text{EE}(\text{IC})$ and $\text{EE}(\text{VCO}_2)$ estimations are both derived from the metabolic monitor. Differences between $\text{EE}(\text{IC})$ and $\text{EE}(\text{VCO}_2)$ must be either due to an incorrect assumption about RQ or due to variations in ventilation. Variations in ventilation will cause different variations in $\text{EE}(\text{IC})$ and $\text{EE}(\text{VCO}_2)$ because the time constant for VCO_2 equilibration is much longer (10–20 min) [27, 28] than the time constant for VO_2 equilibration (2–3 min) [29].

The accuracy of the $\text{EE}(\text{VCO}_2)$ estimates and that of some commonly used predictive equations (Table 1) were compared to $\text{EE}(\text{IC})$.

The cohort-specific value of SF for the Harris–Benedict equation (b, Table 1) was calculated using the following equation:

$$\text{SF} = \text{mean EE}(\text{IC}) / \text{mean EE}(\text{HB}) \quad (5)$$

The SF for methods c and d (Table 1) were similarly determined using their respective mean EE. The result is that the mean EE for the 18 patients determined by each method equals the mean $\text{EE}(\text{IC})$ determined by Eq. 2 (the reference method).

The ideal body mass (IBM) was calculated from the Hamwi equations [31]:

$$\text{Men: IBM} = 48.0 \text{ kg} + 2.7 \text{ kg} \cdot (\text{height} - 1.524 \text{ m}) / 0.0254 \text{ m} \quad (6)$$

$$\text{Women: IBM} = 45.5 \text{ kg} + 2.2 \text{ kg} \cdot (\text{height} - 1.524 \text{ m}) / 0.0254 \text{ m} \quad (7)$$

Sensitivity analysis of RQ

The practical use of VCO_2 -based calorimetry relies on a choice of RQ. A sensitivity study of the effect of the choice of RQ will be conducted. In six studies [14, 18, 32–36], the average reported cohort values for RQ ranged from 0.76 to 0.89. These minimum and maximum values and the extreme range of the physiological range (0.7–1.0) [23] will be used in the sensitivity analysis.

Statistical analysis

Over-/underestimation

The bias of each method [the predictive equations and $\text{EE}(\text{VCO}_2)$] was expressed by the difference in percent between mean EE for the method and mean $\text{EE}(\text{IC})$. The significance was tested by a two-tailed paired *t* test. The assumption of normal distribution of tested variables was assessed with the Shapiro–Wilk test.

Quality

The root mean square error (RMSE) was used to describe the quality of the predictions for each method. A comparison of $\text{EE}(\text{VCO}_2)$ and each predictive equation was performed by an *F* test over the prediction errors relative to $\text{EE}(\text{IC})$.

Accuracy

Per-patient EE estimates were defined as accurate if the estimate was within $\pm 10\%$ of the IC measurement. The

Table 1 Predictive equations for estimation of EE

Method	Equation
a	ACCP
	The ACCP equation [9, 10, 30] using BM as the only variable $\text{EE}(\text{ACCP}) = 25 \text{ kcal/kg/day} \cdot \text{BM}$
b	Harris–Benedict
	The Harris–Benedict equation from 1919 [11] multiplied by a SF Men: $\text{EE}(\text{HB}) = (66.5 + 13.75 \text{ kg}^{-1} \cdot \text{BM} + 5.003 \text{ cm}^{-1} \cdot \text{height} - 6.775 \text{ year}^{-1} \cdot \text{age}) \text{ kcal/day} \cdot \text{SF}$ Women: $\text{EE}(\text{HB}) = (655.1 + 9.563 \text{ kg}^{-1} \cdot \text{BM} + 1.85 \text{ cm}^{-1} \cdot \text{height} - 4.676 \text{ year}^{-1} \cdot \text{age}) \text{ kcal/day} \cdot \text{SF}$
c	Harris–Benedict IBM
	The Harris–Benedict equation with ideal body mass (IBM) multiplied by a SF Men: $\text{EE}(\text{HBI}) = (66.5 + 13.75 \text{ kg}^{-1} \cdot \text{IBM} + 5.003 \text{ cm}^{-1} \cdot \text{height} - 6.775 \text{ year}^{-1} \cdot \text{age}) \text{ kcal/day} \cdot \text{SF}$ Women: $\text{EE}(\text{HBI}) = (655.1 + 9.563 \text{ kg}^{-1} \cdot \text{IBM} + 1.85 \text{ cm}^{-1} \cdot \text{height} - 4.676 \text{ year}^{-1} \cdot \text{age}) \text{ kcal/day} \cdot \text{SF}$
d	Mifflin St Jeor
	The Mifflin St Jeor equation [12] multiplied by a SF Men: $\text{EE}(\text{MSJ}) = (9.99 \text{ kg}^{-1} \cdot \text{BM} + 6.25 \text{ cm}^{-1} \cdot \text{height} - 4.92 \text{ year}^{-1} \cdot \text{age} + 166) \text{ kcal/day} \cdot \text{SF}$ Women: $\text{EE}(\text{MSJ}) = (9.99 \text{ kg}^{-1} \cdot \text{BM} + 6.25 \text{ cm}^{-1} \cdot \text{height} - 4.92 \text{ year}^{-1} \cdot \text{age} - 161) \text{ kcal/day} \cdot \text{SF}$
e	Penn State 1
	The original Penn State equation from 1998 [13] $\text{EE}(\text{PS1}) = 1.1 \cdot \text{HB} + (32 \text{ min l}^{-1} \cdot \text{MV} + 140 \text{ }^{\circ}\text{C}^{-1} \cdot T_{\text{Max}} - 5340) \text{ kcal/day}$
f	Penn State 2
	Version 2 of the Penn State equation from 2003 [14] $\text{EE}(\text{PS2}) = 0.85 \cdot \text{HB} + (33 \text{ min l}^{-1} \cdot \text{MV} + 175 \text{ }^{\circ}\text{C}^{-1} \cdot T_{\text{Max}} - 6433) \text{ kcal/day}$
g	Penn State 3
	Version 3 of the Penn State equation from 2003 [14] $\text{EE}(\text{PS3}) = 0.96 \cdot \text{MSJ} + (31 \text{ min l}^{-1} \cdot \text{MV} + 167 \text{ }^{\circ}\text{C}^{-1} \cdot T_{\text{Max}} - 6212) \text{ kcal/day}$

ACCP American College of Chest Physicians, T_{Max} maximum body temperature in 24 h ($^{\circ}\text{C}$)

number of patients with accurate predictions was compared between $\text{EE}(\text{VCO}_2)$ and each predictive equation using Fisher's exact test.

Significance level for all tests was $p < 0.05$. SPSS version 23 was used for statistical analyses.

Qualitative analysis of dynamic errors

Both IC and VCO_2 -based calorimetry rely on the assumption that the rate of ventilated O_2 and CO_2 is reflecting the rate of O_2 consumption and CO_2 production, respectively. However, $\text{EE}(\text{IC})$ and $\text{EE}(\text{VCO}_2)$ calculated from instantaneous values of VO_2 and VCO_2 may be erroneous in situations where respiratory VO_2 and VCO_2 are not equal to the metabolically consumed or produced VO_2 and VCO_2 , respectively. This may occur when the patient's metabolism changes rapidly, or due to external changes to the patient's ventilation. Patients were divided into a group with varying EE and a group with constant EE, according to the method described below. For a patient in each group, a descriptive analysis of the reasons for errors was performed by inspection of the 30-min recordings of MV, VCO_2 , VO_2 and ET-CO_2 and comparing these to the changes in $\text{EE}(\text{IC})$ and $\text{EE}(\text{VCO}_2)$.

Quantitative analysis of dynamic errors

The effects of changes in ventilation were analyzed for both $\text{EE}(\text{IC})$ and $\text{EE}(\text{VCO}_2)$ to compare the two methods' vulnerability to changes in ventilation. For each patient, the maximum deviation of EE from the mean EE was calculated for both $\text{EE}(\text{IC})$ and $\text{EE}(\text{VCO}_2)$. The effect of a 5-min moving average on the calculated EE was explored by comparing the maximum EE deviations from mean EE, for both $\text{EE}(\text{IC})$ and $\text{EE}(\text{VCO}_2)$, before and after its application.

Method for assessing constancy of EE in individual patients
Each patient was analyzed for changes in EE during the 30-min recording period. The chosen marker for this analysis was VO_2 . $\text{EE}(\text{IC})$ is reliant on VCO_2 , and VCO_2 takes 10–20 min to reach steady state following a change in ventilation pattern [27, 28], which implies that VCO_2 and therefore also $\text{EE}(\text{IC})$ may not reflect the metabolically produced VCO_2 for up to 20 min. Thus, both $\text{EE}(\text{IC})$ and VCO_2 are unsuitable as markers for this analysis. VO_2 , however, reaches steady state after 2–3 min [29], implying that metabolic consumption of VO_2 is equal to VO_2 removed from inspired air. As this is a short period, compared with the 30-min recording period, VO_2 was chosen as a metabolic marker for constant EE.

For each patient, the trend line for the VO_2 recording was compared with the average VO_2 over the recording

period. If the difference between the trend line and the average was less than 10 % of the average VO_2 , the patient was considered to have constant EE throughout the recording period.

Results

Comparing estimates of energy expenditure

Eighteen patients (mean age 61 ± 17 years, five women) were included. Average VO_2 for the 18 patients was 343 ± 77 ml/min and average VCO_2 was 273 ± 63 ml/min, giving an average RQ of 0.81. The mean FiO_2 was 42 % with no patient exceeding 50 %. All patients received intravenous glucose during the measurement period, and patients 1, 2, 3, 14, 17 and 18 received enteral nutrition. The mean RQ for the patients receiving enteral nutrition (0.86) was significantly higher ($p < 0.05$; t test, unpaired, two-tailed) than the mean RQ (0.79) for the patients not receiving enteral nutrition. Individual patient characteristics are given in Table 2.

In summary, all predictive equations, a through g, largely over- and underestimated the reference EE value. The bias was the highest for the Penn State equations and the ACCP, while the ranges of estimation difference were largest for the ACCP, Harris–Benedict and Mifflin St Jeor equations (Table 3). The use of SF in the Harris–Benedict and Mifflin St Jeor equations resulted in these equations having a bias of 0 %; however, the quality of prediction was poor for all predictive equations, as reflected by a RMSE of 15 % or greater. Finally, the accuracy was also very poor for all predictive equations, with 50 % or less of patients having accurate EE estimates (Fig. 1).

The $\text{EE}(\text{VCO}_2)$ was significantly better than the predictive equations with a low and acceptable bias. The mean $\text{EE}(\text{VCO}_2)$, with an RQ value of 0.81, was not significantly different from mean $\text{EE}(\text{IC})$, and the $\text{EE}(\text{VCO}_2)$ had a good quality of prediction with an RMSE of 7 %. The $\text{EE}(\text{VCO}_2)$ was accurate in 89 % of the patients, significantly better than the predictive equations. It also had the narrower range of estimation differences (Fig. 1).

Sensitivity analysis of RQ

The sensitivity analysis showed that as long as the RQ is chosen within the published range of average cohort values, 0.76–0.89, the VCO_2 -based calorimetry performs better than the predictive equations.

Analysis of dynamic errors in $\text{EE}(\text{IC})$ and $\text{EE}(\text{VCO}_2)$

As explained earlier, changes in ventilation or rapid changes in patient metabolism can be causes of error in EE estimation. These errors will be described qualitatively and quantitatively.

Table 2 Patient data

Pt. no.	Age (years)	Height (cm)	Gender	BM (kg)	Meas. (h)	VO ₂ (ml/min)	VCO ₂ (ml/min)	RQ	MV (l/min)	T _{Max} (°C)	Vent. mode	Diagnosis	Apache2 score	Sedation
1	54	165	F	65	54	230	209	0.90	12.0	36.5	PS	S	18	No
2	55	165	M	60	44	189	159	0.85	7.4	34.1	VC	S	12	No
3	76	165	M	70	26	365	298	0.82	13.3	38.0	VC	T _{ES}	22	No
4	52	180	M	75	13	373	282	0.76	10.5	37.0	PS	S	17	Se
5	22	180	M	75	20	450	349	0.77	16.1	37.3	VC	S	14	An
6	60	179	M	73	1	294	228	0.77	6.9	35.1	VC	ES	6	Se
7	62	179	M	94	2	416	313	0.76	9.7	36.0	VC	SS	5	An
8	67	172	M	64	1	359	206	0.73	8.0	35.9	PS	SS	20	An
9	73	158	F	69	1	246	193	0.79	7.1	35.4	VC	SS	20	An
10	79	175	M	75	18	407	330	0.81	9.0	37.8	VC	ES	28	Se
11	56	173	M	105	1	416	371	0.89	12.0	35.5	VC	SS	16	An
12	81	155	F	84	1	248	223	0.90	6.4	36.5	VC	SS	12	An
13	82	180	M	100	19	389	310	0.80	12.4	37.1	PS	ES	17	Se
14	74	160	F	70	120	281	217	0.77	7.3	38.0	VC	ES	18	An
15	72	160	M	72	2	347	266	0.77	8.3	36.5	VC	SS	5	An
16	35	176	M	54	18	401	274	0.69	11.6	37.1	VC	ES	16	Se
17	55	170	M	75	72	351	335	0.96	12.0	37.8	VC	ES	29	Se
18	38	165	F	80	96	417	344	0.83	11.3	38.0	PS	T	11	An
Mean	61	170	–	76	28	343	273	0.81	10.1	36.6	–	–	15.9	–
SD	17	8.4	–	13	36	77	63	0.07	2.7	1.1	–	–	6.8	–

Meas: Time from ICU admittance to ICU measurement, VC measurement, PS pressure support, ES volume control, SS scheduled surgery, S sepsis/septic shock, T trauma, No no sedation, Se sedation, An anesthesia

Table 3 Comparison of EE estimates to IC including sensitivity of EE(VCO₂) reliance on RQ

Equation	Mean EE (bias) (kcal/day)	SF	Range of estimation differences	RMSE of EE difference	# Of patients with accurate EE estimates (%)
ACCP	1889 (−20 %)*	NA	[−49 %; 22 %]	28 % [†]	6 (33 %) [‡]
Harris–Benedict	2347 (0 %)	1.55	[−20 %; 61 %]	16 % [†]	9 (50 %) [‡]
Harris–Benedict, IBM	2347 (0 %)	1.67	[−23 %; 76 %]	18 % [†]	8 (35 %) [‡]
Mifflin St Jeor	2347 (0 %)	1.59	[−18 %; 68 %]	15 % [†]	9 (50 %) [‡]
Penn State 1	1782 (−24 %)*	NA	[−41 %; 0 %]	27 % [†]	1 (6 %) [‡]
Penn State 2	1572 (−33 %)*	NA	[−49 %; −10 %]	35 % [†]	1 (6 %) [‡]
Penn State 3	1637 (−30 %)*	NA	[−43 %; −9 %]	32 % [†]	1 (6 %) [‡]
EE(VCO ₂) RQ = 0.81	2332 (−1 %)	NA	[−13 %; 14 %]	7 %	16 (89 %)
EE(IC)	2347 (0 %)	NA	—	—	—
Sensitivity analysis of RQ					
EE(VCO ₂) RQ = 0.70	2626 (12 %)*	NA	[−2 %; 30 %]	12 %	9 (50 %) [‡]
EE(VCO ₂) RQ = 0.76	2455 (5 %)*	NA	[−8 %; 20 %]	8 %	14 (78 %)
EE(VCO ₂) RQ = 0.85	2244 (−4 %)	NA	[−16 %; 10 %]	6 %	16 (89 %)
EE(VCO ₂) RQ = 0.89	2163 (−8 %)*	NA	[−19 %; 6 %]	10 %	10 (56 %)
EE(VCO ₂) RQ = 1.00	1976 (−16 %)*	NA	[−26 %; −3 %]	17 %	4 (22 %) [‡]

The bias in percent is relative to the mean EE(IC). The range of estimation differences is the maximum and minimum difference between the equations and individual mean EE(IC). The RMSE of EE difference is the root mean square error of EE difference between the equations and the IC measurements. Accurate EE estimates are defined as per-patient mean EE within $\pm 10\%$ of EE(IC)

* Significantly different from mean EE(IC)

[†] Significantly greater variance than EE(VCO₂) RQ = 0.81

[‡] Significantly different from EE(VCO₂) RQ = 0.81

Checking for constant EE

Out of the 18 patients, 17 were determined to have constant EE during the 30-min recording period, as the difference between VO₂ trend line and mean was less than 10 %. For patients 1–17, the maximal deviation of the trend line from the mean was between 0.9 and 8 %. Only patient 18 had a major increase in metabolism with the VO₂ trend line deviating 39 % from the mean.

Dynamic errors in patients with variable EE

Figure 2a shows that for patient 18 the MV, VO₂ and VCO₂ are almost constant until 16 min where the patient apparently is aroused and all three parameters rise. VO₂ increases by 78 % from 320 ml/min to about 570 ml/min and remains increased for over 10 min. If the increase had been due to the increased MV, without any increase in metabolism, then VO₂ would have returned to its initial value of about 320 ml/min within 2–3 min. Since this does not happen, the prolonged increase in VO₂ must therefore reflect an increase in metabolism.

Figure 2b shows that both EE(IC) and EE(VCO₂), calculated from the recorded VO₂ and VCO₂, indicate increased EE, approximately to the same degree and simultaneously.

Dynamic errors in patients with constant EE

Most of the 17 patients with constant metabolism had one or more changes of ventilation. Patient 16, whose

VO₂ trend line deviated 2.7 % from the mean VO₂, will be used as an example. The patient, who was volume controlled, had two changes in ventilation (Fig. 3a): a 3-min period of unstable MV from 7.5 to 10.5 min and a sustained reduction in MV from 10 min until the end of the recording.

During the unstable period, MV reached a peak value which is 36 % higher than the steady-state value up to 7.5 min. This gave rise to increases in VO₂ and VCO₂ of 22 and 34 %, respectively, which were mirrored as increases in EE(IC) and EE(VCO₂) of about the same size, 24 and 35 %, respectively (Fig. 3b).

The second change in ventilation was a sustained reduction in MV at 10.5 min from 13.5 to 11.7 l/min. As a result of the reduced ventilation, ET-CO₂ rises, but does not quite reach steady state, because of its 10- to 20-min equilibration time constant. For the same reason, VCO₂ remains low, but rises slowly from 10.5 min and on. In contrast to VCO₂, VO₂ equilibrates within a few minutes and returns to its original value of about 400 ml/min, indicating that there is no reason to suspect that the patient's EE changes during the 10-min period shown in Fig. 3. Therefore, the fluctuations of EE(IC) and EE(VCO₂) must be ascribed to the fluctuations of MV.

The changes in VO₂ and VCO₂ are reflected in the changes in EE(IC) and EE(VCO₂) (Fig. 3b). At 12.5 min, EE(IC) has almost recovered and reached its original

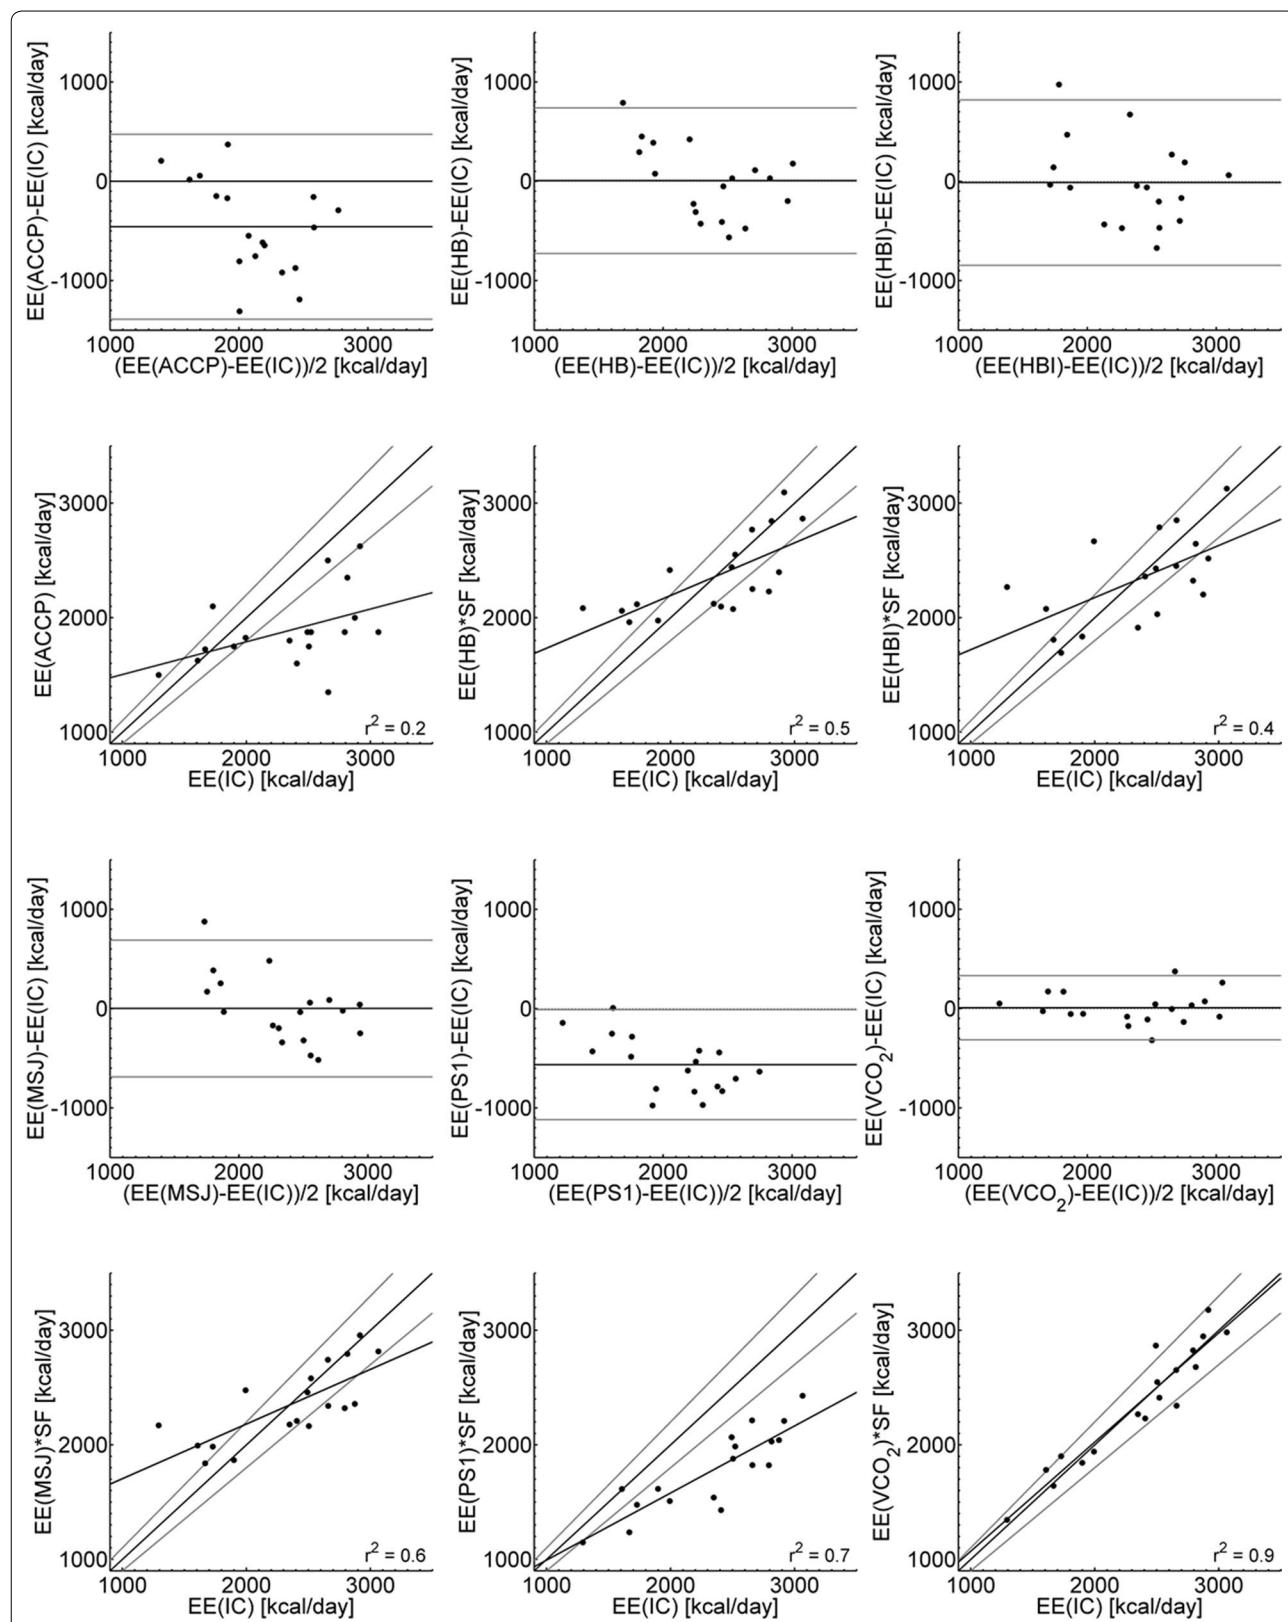


Fig. 1 Bland-Altman plots and scatterplots for predictive equations and VCO_2 -based calorimetry compared with EE estimated using IC. Bland-Altman plots include 95 % limits of agreement. Scatterplots include lines marking $\pm 10\%$ of EE(IC) and linear regression lines with r^2 values

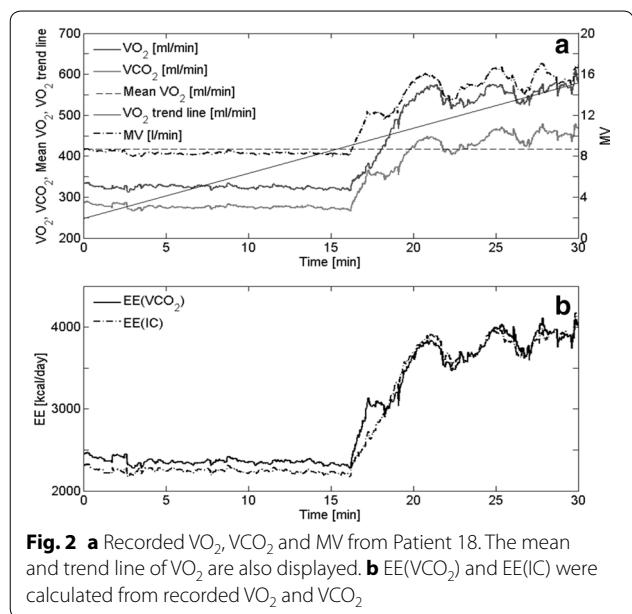


Fig. 2 a Recorded VO_2 , VCO_2 and MV from Patient 18. The mean and trend line of VO_2 are also displayed. b EE(VCO_2) and EE(IC) were calculated from recorded VO_2 and VCO_2

value of 2720 kcal/day. EE(VCO_2) remains low, although it increases slowly.

The conclusion on this qualitative analysis is that rapid changes in MV (a rise or fall with a duration of less than 1 min) are reflected about equally in EE(IC) and EE(VCO_2), that during maintained changes in MV, EE(IC) largely recovers within a few minutes and that EE(VCO_2) will take 10–20 min or more to recover.

Quantitative analysis of dynamic errors

The effect of changes in ventilation is given in Table 4 for each of the 17 patients with stable ventilation. It can be seen that both EE(IC) and EE(VCO_2) are vulnerable to changes in ventilation. EE(IC) has up to 42 % deviation (Patient 8), and EE(VCO_2) has up to 46 % (Patient 16) deviation. EE(IC) and EE(VCO_2) are about equally vulnerable with no significant differences (*t* test) between the mean of the max values for the two methods. In clinical practice, this implies that an instantaneous reading of EE(IC) and EE(VCO_2) cannot safely be used to assess EE.

Applying a 5-min moving average to the calculated EE(IC) reduced the max deviation to 18 % (Table 4, column 3, Patient 10) and the SD of the mean to 7.5 %. For EE(VCO_2), the max deviation was reduced to 14 % (Table 4, column 5, patient 10) and the SD of the mean to 7.3 %.

This means that the introduction of a 5-min running average reduced the dynamic error of the EE(VCO_2) to a size comparable to the RMSE of EE difference (Table 3).

Discussion

The goal of this study was to investigate the accuracy of EE estimates by predictive equations and by VCO_2 -based

calorimetry in a small cohort of critically ill patients, most of them soon after admission to the ICU. The results corroborate the previously reported [6, 15] inaccuracy of predictive equations for EE. Tatucu-Babet et al. [6] found underestimations of EE up to 41 % and overestimations up to 66 %, which is similar to the results in this study. In our study, even the best of the equations, the Mifflin St Jeor equation, was accurate only in 50 % of the patients.

The two predictive equations with the best performance in our study were Mifflin St Jeor and Harris–Benedict. Both of these equations have the methodological problem that they require a SF to account for the increased metabolism following an insult. The SFs giving the best fit to our data were 1.59 and 1.55 for the two equations, respectively. Published mean values for SF for different cohorts range from 1.13 to 1.6 [6], and our cohort values for SF thus fall close to the upper end of the published range. This may partially be due to statistical fluctuations due to our small number of patients, but in general the large range of reported SF implies that SF used must be adapted to the cohort of patients. An additional problem is that EE, and thus SF, tends to increase for the first 9–11 days [16, 17] after the insult that led to the admission to the ICU.

In our small sample of ICU patients, VCO_2 -based calorimetry estimated EE accurately in most patients (89 %), even in cases where ventilation was changing during the recording period. VCO_2 -based calorimetry performed significantly better than all predictive equations in agreement with earlier findings both in adults and in children [21, 22].

However, VCO_2 -based calorimetry has two methodological challenges. The first is that the method requires a choice of RQ to be made, and the second is that the accuracy of the estimation is affected by instant variability in measurements of MV and VCO_2 .

RQ was fitted to our cohort by choosing the average value of RQ for the cohort in the calculation of EE(VCO_2). In practice, the value of RQ for the cohort will not be available, and the robustness of VCO_2 -based calorimetry was explored by a sensitivity analysis. The analysis showed that for any choice of RQ within the published range of cohort values for RQ (0.76–0.89) [14, 18, 32–36], the EE(VCO_2) equation performed significantly better than the predictive equations. The results of the sensitivity analysis show that as long as the RQ value chosen by the clinician is within the published range of values, the estimation of EE will be better compared with predictive equations.

The use of nutritional RQ has been explored both in children [21] and in adults [22], and both failed to provide evidence that EE estimates are improved by using

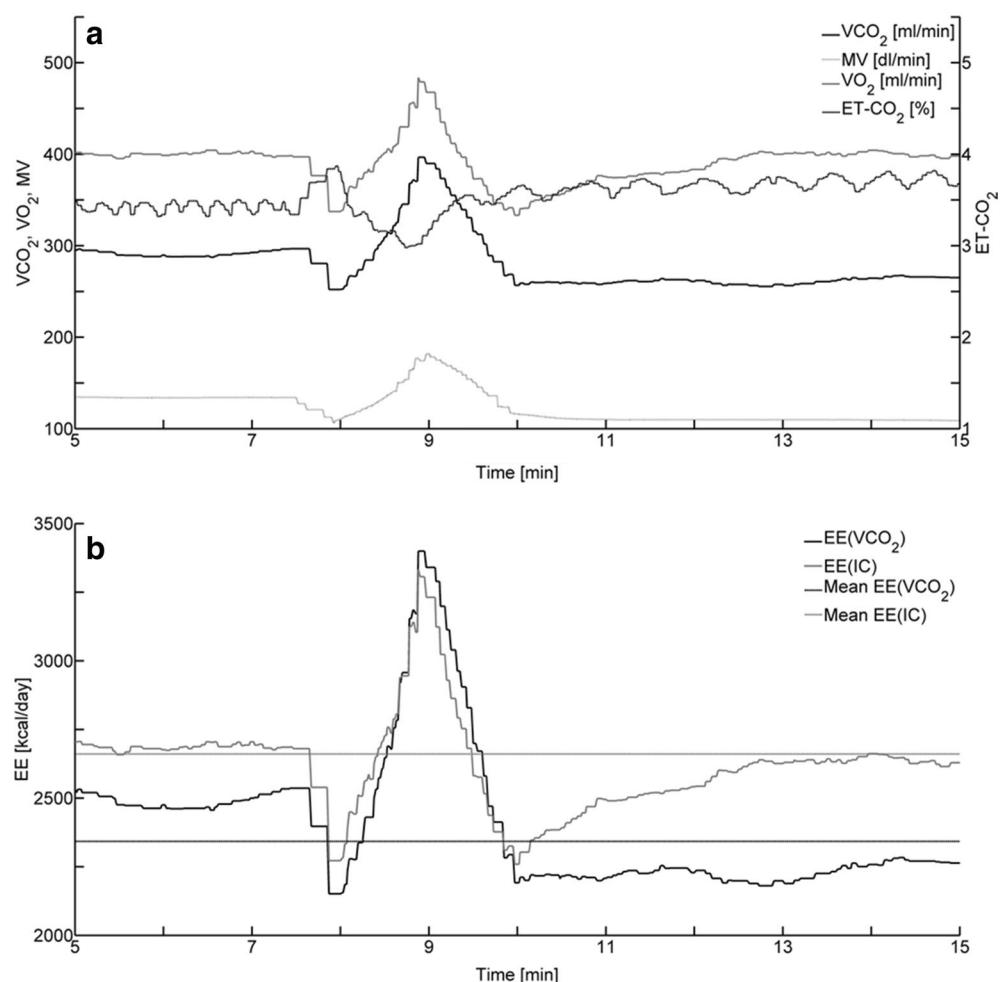


Fig. 3 **a** Recorded values from Patient 16 of VCO_2 , ET-CO_2 , VO_2 and MV. **b** EE(VCO_2) and EE(IC) calculated from recorded VO_2 and VCO_2 , including means of EE(VCO_2) and EE(IC)

nutritional RQ. In children [21], the nutritional RQ gave poorer estimates than the mean RQ for the cohort. For the patients in our cohort, a nutrition-based RQ would have given poorer accuracy, as evidenced by the observation that contrary to expectations the patients receiving only glucose had a significantly lower RQ than the patients also receiving enteral nutrition. An explanation of the failure of nutritional RQ to improve EE estimates may be due to the mobilization of the patient's own energy stores in the early catabolic phase of critical illness, where plasma concentrations of glucose, fatty acids and amino acids are strongly increased, thus weakening the link between nutrition and metabolism [16, 17].

If a suggestion is to be made on a choice of RQ for VCO_2 -based calorimetry, the authors suggest 0.85 as this number is in the middle of the physiological range (0.7–1.0); is within the published range of cohort values for

RQ (0.76–0.89); gives an acceptable –4 % mean EE difference from IC; gives the smallest RMSE (6 %); and is the highest number of accurate EE estimates in this cohort.

The second methodological problem with VCO_2 -based calorimetry is that EE(VCO_2) is inaccurate during and immediately after changes in MV. A qualitative analysis showed that instant values of EE(IC) were almost as vulnerable to fluctuations in MV as EE(VCO_2) with fluctuations about the same size as the fluctuations in MV. This behavior is compatible with the 10- to 20-min time constant for VCO_2 equilibration, supported by both mathematical models of VCO_2 storage and transport [28] and experimental data [27]. The problems arising from fluctuations in MV and thus VCO_2 and VO_2 are less pronounced when using IC as the equilibration time for VO_2 is 2–3 min, and as can be seen from Eq. (2), VO_2 has the larger influence on the EE estimation. Smoothing

Table 4 Maximal deviations from mean EE and from a mean of EE after the inclusion of a 5-min running average of EE, for both EE(IC) and EE(VCO₂)

	Max EE(IC) versus EE(IC) (%)	Max EE(IC) versus 5-min EE(IC) (%)	Max EE(VCO ₂) versus EE(VCO ₂) (%)	Max EE(VCO ₂) versus 5-min EE(VCO ₂) (%)
1	-7	-2	-11	-3
2	22	-12	-20	-13
3	12	-6	14	-5
4	-20	4	-21	8
5	-4	1	-5	1
6	-4	-3	-2	-1
7	15	5	-7	4
8	42	11	-38	11
9	11	9	8	-6
10	31	18	-24	14
11	-3	-1	2	1
12	-6	-3	-3	2
13	20	4	5	2
14	-7	-2	-6	-3
15	-9	13	-9	11
16	-28	9	46	12
17	11	4	17	7
Mean (±SD)	4.4 (±18.3)	2.8 (±7.5)	-3.2 (±18.9)	2.5 (±7.3)
RMS	18	8	19	8

Deviations are expressed as a percentage of the mean EE

EE(VCO₂) and EE(IC) with a 5-min running average reduced the sensitivity to fluctuations in MV and reduced the RMSE of the maximum deviations from 19 and 18 %, respectively, to 8 % for both of them. Although a 5-min average thus substantially reduced the variability of EE(VCO₂) and EE(IC), it is still advisable to avoid using measurements taken during fluctuations or up to 20 min after changes in MV to allow for equilibration of VCO₂. Alternatively 24-h measurements of VCO₂ could be used in the VCO₂-based calorimetry. Using the mean 24-h value has benefits over a 30-min measurement period as the influence of fluctuations from hypo- or hyperventilation on EE(VCO₂) and EE(IC) is eliminated, reducing the discrepancy between metabolic production and pulmonary uptake or excretion.

The widespread availability and relatively low cost of capnometers, and software to analyze VCO₂ from CO₂ concentrations and expiratory volume, may make VCO₂-based calorimetry a simple and accurate method for determination of EE in critically ill patients, whenever needed. Production of the most extensively used IC system (Deltatrac Metabolic Monitor) has been discontinued, and newer available IC systems give conflicting EE estimates [37]. Thus, in the absence of other devices validated for use in the ICU, use of CO₂-based calorimetry

can represent a useful alternative for the determination of EE.

Abbreviations

EE: energy expenditure; VO₂: measured oxygen consumption; VCO₂: measured carbon dioxide production; IC: indirect calorimetry; BM: body mass; MV: minute volume; SF: stress factor; RQ: respiratory quotient; N: nitrogen metabolism.

Authors' contributions

MHH-P, SA and J-CP contributed to conception and design of the research; MHH-P and J-CP contributed to the acquisition of the data; all authors contributed to the analysis and interpretation of the data and drafting of the manuscript, critically revised the manuscript and agree to be fully accountable for ensuring the integrity and accuracy of the work. All authors read and approved the final manuscript.

Author details

¹ Center for Model-based Medical Decision Support (MMDS), Department of Health Science and Technology, Aalborg University, Fredrik Bajers Vej 7E, 9220 Aalborg East, Denmark. ² Department of Intensive Care, Erasme University Hospital, Université Libre de Bruxelles, 808 Route de Lennik, 1070 Brussels, Belgium.

Competing interests

The study was funded by the respective institutions of the authors, without external financial support, and the authors declare that they have no competing interests.

Received: 28 October 2015 Accepted: 8 February 2016

Published online: 18 February 2016

References

1. Fraipont V, Preiser JC. Energy estimation and measurement in critically ill patients. *J Parenter Enteral Nutr.* 2013;37(6):705–13.
2. Preiser JC, van Zanten AR, Berger MM, Biolo G, Casaer MP, Doig GS, et al. Metabolic and nutritional support of critically ill patients: consensus and controversies. *Crit Care.* 2015;19(1):35.
3. Weir JdV. New methods for calculating metabolic rate with special reference to protein metabolism. *J Physiol (Lond).* 1949;109(1–2):1–9.
4. Davis KA, Kinn T, Esposito TJ, Reed RL 2nd, Santaniello JM, Luchette FA. Nutritional gain versus financial gain: the role of metabolic carts in the surgical ICU. *J Trauma.* 2006;61(6):1436–40.
5. Cheng C, Chen C, Wong Y, Lee B, Kan M, Huang Y. Measured versus estimated energy expenditure in mechanically ventilated critically ill patients. *Clin Nutr.* 2002;21(2):165–72.
6. Tatuću-Babet OA, Ridley EJ, Tierney AC. The prevalence of underprescription or overprescription of energy needs in critically ill mechanically ventilated adults as determined by indirect calorimetry: a systematic literature review. *J Parenter Enteral Nutr.* 2016;40(2):212–25.
7. Heidegger CP, Berger MM, Graf S, Zingg W, Darmon P, Costanza MC, et al. Optimisation of energy provision with supplemental parenteral nutrition in critically ill patients: a randomised controlled clinical trial. *Lancet.* 2013;381(9864):385–93.
8. Cerra FB, Benitez MR, Blackburn GL, Irwin RS, Jeejeebhoy K, Katz DP, et al. Applied nutrition in ICU patients: a consensus statement of the American College of Chest Physicians. *CHEST J.* 1997;111(3):769–78.
9. Kreymann KG, Berger MM, Deutz NE, Hiesmayr M, Jolliet P, Kazandjiev G, et al. ESPEN guidelines on enteral nutrition: intensive care. *Clin Nutr.* 2006;25:210–23.
10. Heyland DK, Dhaliwal R, Drover JW, Gramlich L, Dodek P, Canadian Critical Care Clinical Practice Guidelines Committee. Canadian clinical practice guidelines for nutrition support in mechanically ventilated, critically ill adult patients. *J Parenter Enteral Nutr.* 2003;27(5):555–73.
11. Harris JA, Benedict FG. A biometric study of human basal metabolism. *Proc Natl Acad Sci USA.* 1918;4(12):370–3.
12. Mifflin MD, St Jeor ST, Hill LA, Scott BJ, Daugherty SA, Koh YO. A new predictive equation for resting energy expenditure in healthy individuals. *Am J Clin Nutr.* 1990;51(2):241–7.
13. Frankenfield D. Energy dynamics. In: LE Matarese GM, editor. *Contemporary nutrition support practice: a clinical guide* Philadelphia. Philadelphia: W.B. Saunders Company; 1998. p. 79–98.
14. Frankenfield D, Smith JS, Cooney RN. Validation of 2 approaches to predicting resting metabolic rate in critically ill patients. *J Parenter Enteral Nutr.* 2004;28(4):259–64.
15. Frankenfield D, Roth-Yousey L, Compher C, Evidence Analysis Working Group. Comparison of predictive equations for resting metabolic rate in healthy nonobese and obese adults: a systematic review. *J Am Diet Assoc.* 2005;105(5):775–89.
16. Plank LD, Hill GL. Sequential metabolic changes following induction of systemic inflammatory response in patients with severe sepsis or major blunt trauma. *World J Surg.* 2000;24:630–8.
17. Monk DN, Plank LD, Franch-Arcas G, Finn PJ, Street SJ, Hill GL. Sequential changes in the metabolic response in critically injured patients during the first 25 days after blunt trauma. *Ann Surg.* 1996;223(4):395–405.
18. Dickerson RN, Gervasio JM, Riley ML, Murrell JE, Hickerson WL, Kudsk KA, et al. Accuracy of predictive methods to estimate resting energy expenditure of thermally-injured patients. *J Parenter Enteral Nutr.* 2002;26(1):17–29.
19. Ortega R, Connor C, Kim S, Djang R, Patel K. Monitoring ventilation with capnography. *N Engl J Med.* 2012;367(19):e27.
20. Rousing ML, Simonsen M, Andreassen S, Pielmeier U, Preiser J. Comparison of resting energy expenditure estimated using predictive equations and measured using indirect calorimetry in critically ill patients. *Intensive Care Med.* 2014;40(Supplement 1):82.
21. Mehta NM, Smallwood CD, Joosten KF, Hulst JM, Tasker RC, Duggan CP. Accuracy of a simplified equation for energy expenditure based on bedside volumetric carbon dioxide elimination measurement—a two-center study. *Clin Nutr.* 2015;34(1):151–5.
22. Stapel SN, de Groot HS, Alimohamad H, Elbers PWG, Girbes ARJ, Weijns PJM, et al. Ventilator-derived carbon dioxide production to assess energy expenditure in critically ill patients: proof of concept. *Crit Care.* 2015;19:370.
23. McClave SA, Lowen CC, Kleber MJ, McConnell JW, Jung LY, Goldsmith LJ. Clinical use of the respiratory quotient obtained from indirect calorimetry. *J Parenter Enteral Nutr.* 2003;27(1):21–6.
24. Knaus WA, Draper EA, Wagner DP, Zimmerman JE. APACHE II: a severity of disease classification system. *Crit Care Med.* 1985;13(10):818–29.
25. Masuda T, Kuramoto M, Tanimoto H, Yamamoto K, Ikeshima S, Kitano Y, et al. Intraoperative baseline oxygen consumption as prognostic factor in emergency open abdominal surgery. *J Crit Care.* 2015. doi:10.1016/j.jcrc.2015.11.014.
26. GE Healthcare. Datex-Ohmeda S/5-modules technical reference manual. 2005.
27. Ivanov S, Nunn J. Influence of duration of hyperventilation on rise time of P_{CO_2} after step reduction of ventilation. *Respir Physiol.* 1968;5(2):243–9.
28. Andreassen S, Rees SE. Mathematical models of oxygen and carbon dioxide storage and transport: interstitial fluid and tissue stores and whole-body transport. *Crit Rev Biomed Eng.* 2005;33(3):265–98.
29. Chiumello D, Coppola S, Froio S, Mietto C, Brazzi L, Carlesso E, et al. Time to reach a new steady state after changes of positive end expiratory pressure. *Intensive Care Med.* 2013;39(8):1377–85.
30. McClave SA, Martindale RG, Vanek VW, McCarthy M, Roberts P, Taylor B, et al. Guidelines for the provision and assessment of nutrition support therapy in the adult critically ill patient: Society of Critical Care Medicine (SCCM) and American Society for Parenteral and Enteral Nutrition (ASPN). *J Parenter Enteral Nutr.* 2009;33(3):277–316.
31. Hamwi G. Therapy: changing dietary concepts. In: Danowski T, editor. *Diabetes mellitus: diagnosis and treatment*, vol. 1. American Diabetes Association; 1964. p. 73–8.
32. Weissman C, Kemper M. CRTT tJA. Resting metabolic rate of the critically ill patient: measured versus predicted. *Anesthesiology.* 1986;64(6):673–9.
33. Weissman C, Kemper M, Elwyn D, Askanazi J, Hyman A, Kinney J. The energy expenditure of the mechanically ventilated critically ill patient. An analysis. *CHEST J.* 1986;89(2):254–9.
34. Faisy C, Guerot E, Diehl JL, Labrousse J, Fagon JY. Assessment of resting energy expenditure in mechanically ventilated patients. *Am J Clin Nutr.* 2003;78(2):241–9.
35. Hanique G, Dugernier T, Laterre P, Dougnac A, Roeseler J, Reynaert M. Significance of pathologic oxygen supply dependency in critically ill patients: comparison between measured and calculated methods. *Intensive Care Med.* 1994;20(1):12–8.
36. Bursztein S, Saphar P, Singer P, Elwyn DH. A mathematical analysis of indirect calorimetry measurements in acutely ill patients. *Am J Clin Nutr.* 1989;50(2):227–30.
37. Sundström M, Tjäder I, Rooyackers O, Werner J. Indirect calorimetry in mechanically ventilated patients. A systematic comparison of three instruments. *Clin Nutr.* 2013;32(1):118–21.