

## Subject-Independent Detection of Movement-Related Cortical Potentials and Classifier Adaptation from Single-Channel EEG

Jochumsen, Mads Røvsing

*Published in:*  
Converging Clinical and Engineering Research on Neurorehabilitation IV

*DOI (link to publication from Publisher):*  
[10.1007/978-3-030-70316-5\\_13](https://doi.org/10.1007/978-3-030-70316-5_13)

*Publication date:*  
2022

*Document Version*  
Accepted author manuscript, peer reviewed version

[Link to publication from Aalborg University](#)

*Citation for published version (APA):*  
Jochumsen, M. R. (2022). Subject-Independent Detection of Movement-Related Cortical Potentials and Classifier Adaptation from Single-Channel EEG. In D. Torricelli, M. Akay, & J. L. Pons (Eds.), Converging Clinical and Engineering Research on Neurorehabilitation IV: Proceedings of the 5th International Conference on Neurorehabilitation (ICNR2020), October 13–16, 2020 (pp. 77-81). Springer. [https://doi.org/10.1007/978-3-030-70316-5\\_13](https://doi.org/10.1007/978-3-030-70316-5_13)

### General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal -

### Take down policy

If you believe that this document breaches copyright please contact us at [vbn@aub.aau.dk](mailto:vbn@aub.aau.dk) providing details, and we will remove access to the work immediately and investigate your claim.



# Subject-Independent Detection of Movement-Related Cortical Potentials and Classifier Adaptation from Single-Channel EEG

Mads Jochumsen

**Abstract**—Brain-computer interfaces have been proposed for stroke rehabilitation, but there are some impeding factors for them to be translated into clinical practice. One of them is the need for calibration. In this study it was investigated if subject-independent calibration is possible for detecting movement-related potentials associated with hand movements, and what the optimal number of movement epochs is to maximize the detection performance. Twelve healthy subjects performed 100 palmar grasps while continuous EEG was recorded. Template matching was performed between movement and idle epochs.  $72\pm 10\%$  of all epochs were correctly classified using the subject-independent approach while  $78\pm 9\%$  of the epochs were correctly classified using the individualized approach. The highest classification accuracies were obtained when using  $54\pm 23$  movement epochs for calibration. In conclusion, it is possible to use a subject-independent approach for detecting movement-related cortical potentials, but the performance is slightly lower compared to individualized calibration.

## I. INTRODUCTION

BRAIN-COMPUTER INTERFACES have been proposed for stroke rehabilitation over the past years. It has been shown in several studies that neural plasticity, the underlying factor of motor recovery, can be induced [1] and gains in functional scores have been reported in stroke patients [2]. A Brain-Computer Interface (BCI) can induce neural plasticity by pairing movement-related brain activity with temporally correlated somatosensory feedback from e.g. electrical stimulation of nerves and muscles or passive movement from rehabilitation robots and exoskeletons [3]. It is not known how strict the temporal association between movement-related activity and inflow of somatosensory feedback has to be. It has been suggested that there should be a very strict timing where the intended movement is predicted [4], while other findings have suggested that such a strict temporal association may not be needed [5]. However, if a strict temporal association is needed, the movement-related activity has to be predicted from single-trial EEG. This is possible through detection of movement-related brain activity that precedes a movement, which can be done from either movement-related cortical potentials (MRCPs) or event-related desynchronization (ERD) [6]. It has been shown in several studies that these two phenomena can be detected from single-trial EEG with accuracies in the range of 70-80% in stroke patients [7]. To be able to utilize this in a BCI, a number of movements (roughly 30-50 movements) needs to

be performed such that a classifier can be trained to discriminate between movement and idle activity. This takes time, especially in a potential rehabilitation scenario where the therapist needs to mount the EEG cap and perform the system calibration. It is likely that this will take too much time for the therapist, and this wasted time may be deducted from the actual training with the patient. To increase the acceptance of a BCI-approach for stroke rehabilitation, it would be ideal if the patient could mount the cap him/herself [8], and that the BCI would not require any calibration, or at least a very low number of movement trials for calibration. It has been shown previously in a couple of studies that ERD [9], [10] and MRCPs [11], [12] can be detected using a global approach where previously recorded data from multiple subjects can be used for calibration hence removing the calibration time. For the MRCP, it has been reported for foot movements. In this study, it will be investigated if similar findings are obtained for hand movements. The aims of this study are to: 1) compare the detection of MRCPs associated with hand movements from single-trial EEG using a global and individualized detector approach, and 2) determine the relationship between detection performance and number of movements used for calibration.

## II. METHODS

### A. Subjects

Twelve healthy subjects participated ( $28\pm 3$ , two females). The subjects gave their written informed consent prior to participation. The local ethical committee (N-20130081) approved all procedures.

### B. Recordings

Nine channels of EEG were recorded from F3, Fz, F4, C3, Cz, C4, P3, Pz and P4 (EEG amplifiers, Nuamps Express, Neuroscan). The channels were referenced to the right mastoid bone and a ground electrode was placed on the forehead. The signals were sampled with 500 Hz. The impedance of the electrodes was below 5 k $\Omega$ .

### C. Experimental Setup

The subjects were seated in a comfortable chair. They performed 100 visually cued ballistic palmar grasps of the right hand. A digital trigger was used to synchronize the visual movement cues with the EEG. The subjects were

This work was funded by VELUX FONDEN (project no. 22357).

M. Jochumsen is with the Department of Health Science and Technology, Aalborg University, Aalborg, Denmark (mj@hst.aau.dk).

instructed to sit as still as possible and minimize blinking and activity of the facial muscles during the recordings. Each movement was separated by a 10-second rest period.

#### D. Data Analysis

Only Cz was used for the data analysis. The raw EEG was bandpass filtered from 0.05 to 5 Hz using a 4<sup>th</sup> order Butterworth filter with zero phase shift and downsampled to 25 Hz to reduce the processing time. The processed continuous signal was divided into two types of trials/epochs 1) movement epochs (from -1.5 to 0.5 s with respect to the task onset), and 2) idle epochs (from -5 to -3 s with respect to the task onset). 100 movement and idle epochs were extracted in total. The mean value of each epoch was subtracted from the respective epoch. To investigate the global approach, a linear discriminant analysis (LDA) classifier was trained on all movement and idle epochs from the subjects that were available except for the test subject (all the epochs from the test subject was used for testing). A template was obtained from all movement epochs (average across epochs), and the autocorrelation was calculated between the template and each epoch, movement and idle. To investigate the effect of the number of movement epochs for the individualized calibration, the first five movement epochs were used to extract a template and to calibrate the LDA, and the remaining epochs were used for testing. The number of epochs was increased by one hence increasing the number of movement epochs for calibration until 20 epochs remained for testing. A paired t-test was performed between the classification accuracies obtained for the global approach and for the highest classification accuracy in the individualized approach.

### III. RESULTS

The results are summarized in Table 1 and Fig. 1.  $72\pm10\%$  (across subjects) of the epochs were correctly classified for the global approach while  $78\pm9\%$  of the epochs were correctly classified in the individualized approach. The accuracies were significantly higher for the individualized approach ( $t_{(11)}=-3.5$ ;  $P=0.005$ ). The highest accuracies in the individualized approach were obtained when  $54\pm23$  movements were performed; however, there is a large standard deviation.

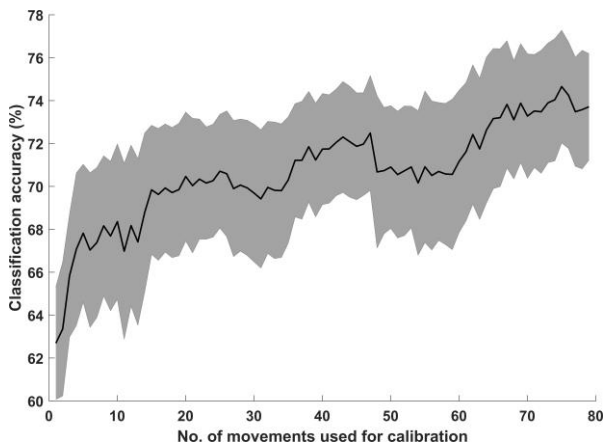


TABLE I  
GLOBAL VS INDIVIDUALIZED CLASSIFICATION

Subject	Global [%]	Individual [%]	No. Epochs for best performance
1	82	86	67
2	79	76	43
3	65	81	65
4	60	71	79
5	69	73	75
6	84	88	64
7	78	76	38
8	69	78	74
9	76	80	59
10	86	91	6
11	61	74	62
12	56	59	18
Mean $\pm$ std	72 $\pm$ 10%	78 $\pm$ 9%	54 $\pm$ 23

Fig. 1. Average and standard error of the classification across subjects for the individualized calibration.

### IV. CONCLUSION

It was possible to use a subject-independent approach for detecting MRCPs associated with hand movements, although the performance was slightly lower compared to the individualized approach. This may have implications for the calibration strategies of MRCP-based BCIs.

### REFERENCES

- [1] R. Xu et al, "A Closed-Loop Brain-Computer Interface Triggering an Active Ankle-Foot Orthosis for Inducing Cortical Neural Plasticity," Biomedical Engineering, IEEE Transactions On, vol. 20, (4), pp. 2092-2101, 2014.
- [2] M. A. Cervera et al, "Brain-computer interfaces for post-stroke motor rehabilitation: a meta-analysis," Annals of Clinical and Translational Neurology, vol. 5, (5), pp. 651-663, 2018.
- [3] M. Jochumsen et al, "Investigation of Optimal Afferent Feedback Modality for Inducing Neural Plasticity with A Self-Paced Brain-Computer Interface," Sensors, vol. 18, (11), pp. 3761, 2018.
- [4] N. Mrachacz-Kersting et al, "Precise temporal association between cortical potentials evoked by motor imagination and afference induces cortical plasticity," J. Physiol. (Lond. ), vol. 590, (7), pp. 1669-1682, 2012.
- [5] M. Jochumsen et al, "EMG-versus EEG-Triggered Electrical Stimulation for Inducing Corticospinal Plasticity," IEEE Transactions on Neural Systems and Rehabilitation Engineering, 2019.
- [6] J. Ibáñez et al, "Detection of the onset of upper-limb movements based on the combined analysis of changes in the sensorimotor rhythms and slow cortical potentials," Journal of Neural Engineering, vol. 11, (5), pp. 056009, 2014.
- [7] M. Jochumsen et al, "Detecting and classifying movement-related cortical potentials associated with hand movements in healthy subjects and stroke patients from single-electrode, single-trial EEG," Journal of Neural Engineering, vol. 12, (5), pp. 056013, 2015.
- [8] M. Jochumsen et al, "Evaluation of EEG Headset Mounting for Brain-Computer Interface-Based Stroke Rehabilitation by Patients, Therapists, and Relatives," Frontiers in Human Neuroscience, vol. 14, 2020.
- [9] S. Fazli et al, "Subject independent EEG-based BCI decoding," Advances in Neural Information Processing Systems, vol. 22, pp. 513-521, 2009.
- [10] M. Krauledat et al, "Towards zero training for brain-computer interfacing," PLoS ONE, vol. 3, (8), 2008.
- [11] I. K. Niazi et al, "Detection of movement-related cortical potentials based on subject-independent training," Med. Biol. Eng. Comput., vol. 51, (5), pp. 507-512, 2013.
- [12] M. Jochumsen et al, "Effect of subject training on a movement-related cortical potential-based brain-computer interface," Biomedical Signal Processing and Control, vol. 41, pp. 63-68, 2018.