



Aalborg Universitet

AALBORG UNIVERSITY
DENMARK

Measuring and monitoring skill learning in closed-loop myoelectric hand prostheses using speed-accuracy tradeoffs

Mamidanna, Pranav; Gholinezhad, Shima; Farina, Dario; Dideriksen, Jakob Lund; Dosen, Strahinja

Published in:
Journal of Neural Engineering

DOI (link to publication from Publisher):
[10.1088/1741-2552/ad2e1c](https://doi.org/10.1088/1741-2552/ad2e1c)

Creative Commons License
CC BY 4.0

Publication date:
2024

Document Version
Publisher's PDF, also known as Version of record

[Link to publication from Aalborg University](#)

Citation for published version (APA):
Mamidanna, P., Gholinezhad, S., Farina, D., Dideriksen, J. L., & Dosen, S. (2024). Measuring and monitoring skill learning in closed-loop myoelectric hand prostheses using speed-accuracy tradeoffs. *Journal of Neural Engineering*, 21(2), Article 026008. <https://doi.org/10.1088/1741-2552/ad2e1c>

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal -

Take down policy

If you believe that this document breaches copyright please contact us at vbn@aub.aau.dk providing details, and we will remove access to the work immediately and investigate your claim.

PAPER • OPEN ACCESS


Measuring and monitoring skill learning in closed-loop myoelectric hand prostheses using speed-accuracy tradeoffs

To cite this article: Pranav Mamidanna *et al* 2024 *J. Neural Eng.* **21** 026008

View the [article online](#) for updates and enhancements.

You may also like

- [Inclusion of thin target and source regions in alimentary and respiratory tract systems of mesh-type ICRP adult reference phantoms](#)
Han Sung Kim, Yeon Soo Yeom, Thang Tat Nguyen *et al.*
- [Estimating speed-accuracy trade-offs to evaluate and understand closed-loop prosthesis interfaces](#)
Pranav Mamidanna, Jakob L Dideriksen and Strahinja Dosen
- [Variations of the Plasma Environment Revealed by the Evolution of the Supra-arcade Fan in the 2017 September 10 Flare](#)
Qiangwei Cai, Jing Ye, Hengqiang Feng *et al.*

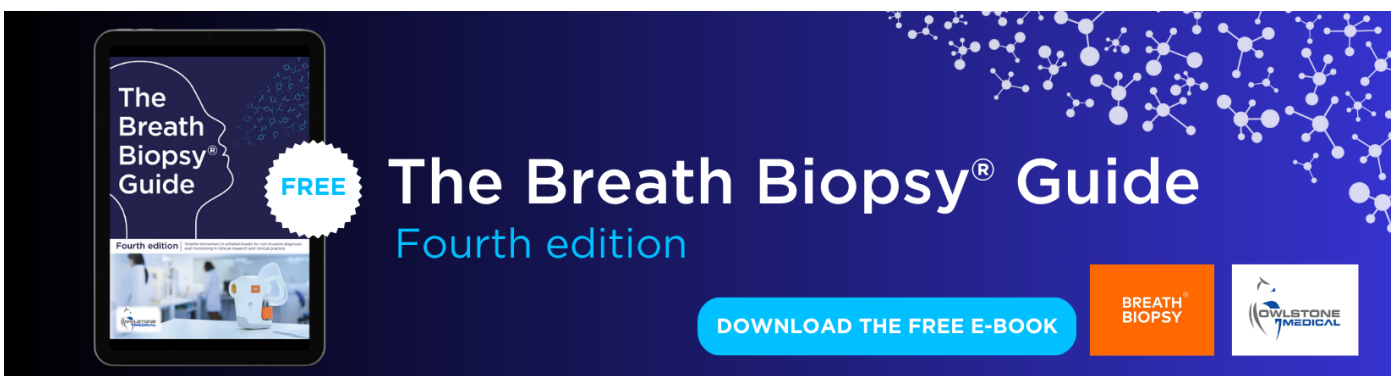

The Breath Biopsy® Guide
Fourth edition

FREE

DOWNLOAD THE FREE E-BOOK

BREATH BIOPSY

OWLSTONE MEDICAL



PAPER

OPEN ACCESS

RECEIVED
10 August 2023

REVISED
29 January 2024

ACCEPTED FOR PUBLICATION
28 February 2024

PUBLISHED
13 March 2024

Original content from
this work may be used
under the terms of the
[Creative Commons
Attribution 4.0 licence](#).

Any further distribution
of this work must
maintain attribution to
the author(s) and the title
of the work, journal
citation and DOI.



Measuring and monitoring skill learning in closed-loop myoelectric hand prostheses using speed-accuracy tradeoffs

Pranav Mamidanna^{1,4} , Shima Gholinezhad^{1,2,4} , Dario Farina³ , Jakob Lund Dideriksen¹ and Strahinja Dosen^{1,*}

¹ Department of Health Science and Technology, Aalborg University, Aalborg, Denmark

² Department of Orthopedic Surgery, Aalborg University Hospital, Aalborg, Denmark

³ Department of Bioengineering, Imperial College London, London, United Kingdom

⁴ These authors contributed equally to this work.

* Author to whom any correspondence should be addressed.

E-mail: sdosen@hst.aau.dk

Keywords: Speed-accuracy trade-off, myoelectric prosthesis control, EMG biofeedback, motor skill acquisition, closed-loop interfaces

Abstract

Objective. Closed-loop myoelectric prostheses, which combine supplementary sensory feedback and electromyography (EMG) based control, hold the potential to narrow the divide between natural and bionic hands. The use of these devices, however, requires dedicated training. Therefore, it is crucial to develop methods that quantify how users acquire skilled control over their prostheses to effectively monitor skill progression and inform the development of interfaces that optimize this process. **Approach.** Building on theories of skill learning in human motor control, we measured speed-accuracy tradeoff functions (SAFs) to comprehensively characterize learning-induced changes in skill—as opposed to merely tracking changes in task success across training—facilitated by a closed-loop interface that combined proportional control and EMG feedback. Sixteen healthy participants and one individual with a transradial limb loss participated in a three-day experiment where they were instructed to perform the box-and-blocks task using a timed force-matching paradigm at four specified speeds to reach two target force levels, such that the SAF could be determined. **Main results.** We found that the participants' accuracy increased in a similar way across all speeds we tested. Consequently, the shape of the SAF remained similar across days, at both force levels. Further, we observed that EMG feedback enabled participants to improve their motor execution in terms of reduced trial-by-trial variability, a hallmark of skilled behavior. We then fit a power law model of the SAF, and demonstrated how the model parameters could be used to identify and monitor changes in skill. **Significance.** We comprehensively characterized how an EMG feedback interface enabled skill acquisition, both at the level of task performance and movement execution. More generally, we believe that the proposed methods are effective for measuring and monitoring user skill progression in closed-loop prosthesis control.

1. Introduction

Myoelectric hand prostheses seek to restore the lost manipulation capabilities of individuals with a limb difference by using electromyographic (EMG) signals to estimate the user's motion intent to drive powered prosthetic devices. Closed-loop user-prosthesis interfaces, which combine EMG-based control and artificial sensory feedback to provide users with a sense of prosthesis state and improve the intuitiveness of

control, hold the promise of bridging the gap between natural and bionic hands [1–3].

To use these sophisticated devices and interfaces, the prospective user needs to train to perform specific, often unintuitive, contractions of their residual muscles. Attaining expert-level skill in user-prosthesis interaction may require guided training over weeks and months [4–6]. This relatively long learning process is due to the inherent variability of EMG-based control and non-linear properties of the prosthesis,

such as non-back-drivability. Quality training is crucial for successful control and poor training has been linked to device rejection [7]. Training is also needed for the feedback side of the interface since the user needs to learn to perceive the sensations artificially elicited [2] and to use this sensation to gain information on the prosthesis state. Quantifying the way and time course of the acquisition of skilled prosthesis control is a fundamental step to developing evidence-based training and rehabilitation protocols [8, 9], designing interfaces that are easier to learn and retain, and understanding the motor learning processes underlying complex human behaviors [10].

Previous studies that investigated prosthesis skill learning, have defined it in terms of improved accuracy, faster movement speed, reduced end-point variability or a combination thereof [8, 9, 11–13]. These studies mainly evaluated skill by asking participants to be as accurate as possible in the given task at a self-chosen comfortable pace, or as fast as possible. However, this approach neglects the effect of the self-chosen speed on the resulting movements and performance. Movement speed and accuracy are fundamentally coupled, and skill can only be inferred when both change in the expected direction [14–18]. Figure 1(A) illustrates this concept with a simple example. If the speed-accuracy measurements over two days for a participant are given by the filled circles as shown in the figure, it would be impossible to dissociate if the improved accuracy (blue circle) is due to better skill or merely due to performing the task at a slower speed (as compared to the gray circle). Consequently, determining speed-accuracy trade-off functions (SAFs, figure 1(A)) has been proposed as a solution to rigorously study skill learning [14, 16, 19].


This approach evaluates task performance systematically and comprehensively by asking the participants to repeat the same task at different speeds. A SAF so measured, characterized by its shape (monotonically increasing), rate, and intercept, succinctly captures skill [20, 21]. Previous work in human motor control demonstrated that SAF changes across days in a way that is consistent across speeds [14, 19], which is mainly driven by better motor execution, reflected by decreased movement variability. However, such a detailed analysis is lacking for prosthesis control—it is unknown if SAF changes such that improvements are similar across speeds, or if some speeds experience larger gains than others (e.g. faster speeds might have larger gains as opposed to slower speeds, simply by having more scope for such gains (figure 1(A), dashed arrows)).

Apart from quantifying skill, SAFs have been used in a recent study to understand and compare how different feedback interfaces afford different speed-accuracy tradeoffs in prosthesis force control [22]. The study demonstrated the relevance of SAFs and

showed how comparing the interfaces at a single speed (corresponding to a single point on the SAF profile), as commonly done in the literature, could generate misleading conclusions. However, it is still unknown how the tradeoff evolves across days during learning, or in other words, how skill develops over time. Quantifying learning-induced changes in the SAF enables us to thoroughly investigate how users acquire skills, and accordingly develop tools to monitor and track skill acquisition and retention.

In relation to the latter, Reis *et al* [14], proposed a model-based method to monitor skill progression. Given that the SAF reflects skill, it follows that if a parametric model of SAF can be obtained, then changes in the parameter values of such a model could be used to monitor skill over time, in a subject-specific manner (figure 1(B)). Notably, they proposed a simple 1-parameter model of SAF such that the single parameter reflected changes in skill. Similarly, Guiard *et al* [23], observed that the SAF in a cursor-pointing task could be captured using a 1-parameter power law model. However, it remains to be seen if such methods generalize to skill monitoring in prosthesis control.

In this study we therefore characterize the SAF resulting from the use of a closed-loop user-prosthesis interface for grip force control, to investigate skill learning and the behavioral changes subserving it. Participants used a closed-loop interface that included a dual-site direct proportional control of prosthesis closing speed and EMG-feedback [24, 25]. In this approach, an array of vibrotactors was employed to deliver the level of the myoelectric signal (prosthesis command input) as the feedback to the participants, thereby facilitating predictive control of grasping force by augmenting a sense of contraction strength. Over the course of 3 days, participants practiced a modified version of the box-and-blocks task where the blocks were required to be grasped at specified forces and speeds (timed force-matching paradigm). We hypothesized that the largest gains in accuracy would be experienced at faster speeds, due to a larger margin for improvement (as explained above) as well as the predictive nature of the feedback. We then built a parametric power-law model of the measured SAFs (figure 1(B)), following previous studies in motor skill learning [14] and human-computer interaction [23, 26]. Using the model, we characterized how the SAF changed across days for this type of closed-loop control interface and compared the results to those reported in the literature for human motor control of natural movements. Finally, we discuss if skill could be inferred from ‘observational’ data, where participants are simply asked to perform the task at their self-chosen comfortable pace to estimate the parameters of the SAF, such that the process of measuring the true SAF could be simplified.

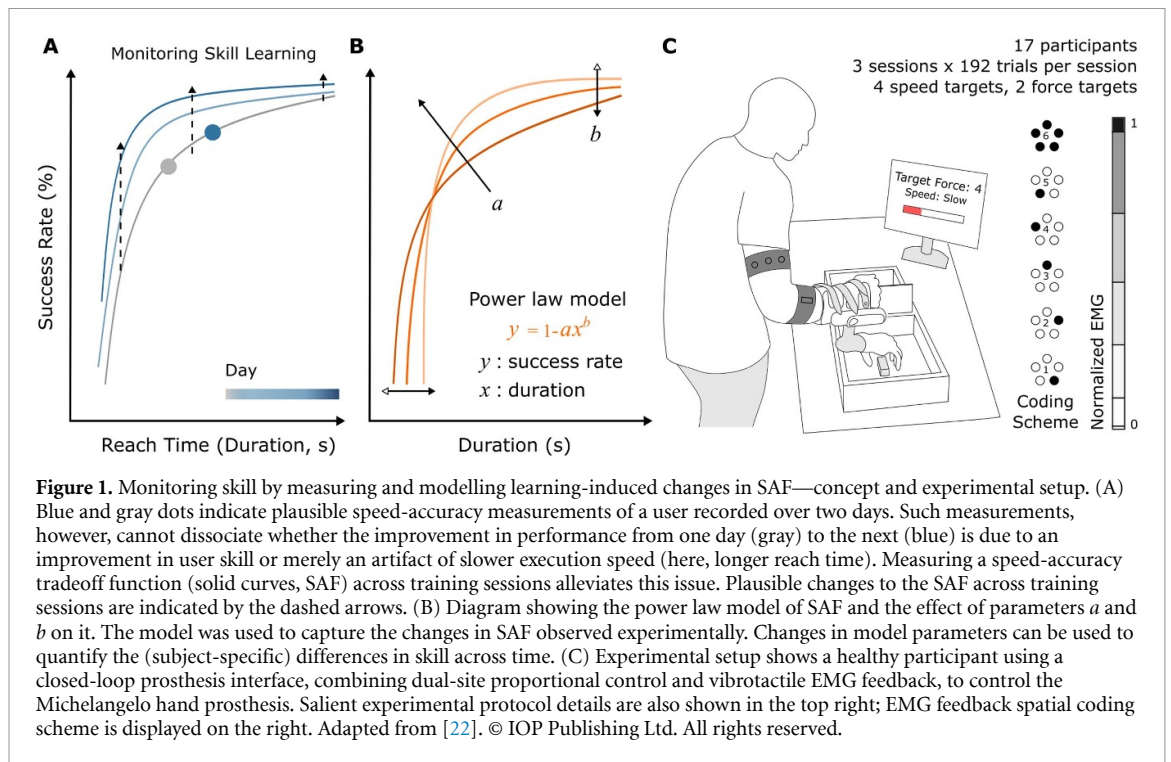

2. Methods

2.1. Participants

Sixteen healthy participants (nine males and seven females with no limb loss, aged 23.5 ± 2.6 years) with no prior experience of myoelectric prosthetic control were recruited. One individual with a transradial limb loss (female, 50 years old, 11 years since traumatic amputation of the non-dominant hand, self-reported to have limited daily use of a single degree of freedom myoelectric prosthesis), who had prior experience with similar experimental setups was also recruited for the study. All participants signed an informed consent form before the start of the experiment. The experimental protocol was approved by the Research Ethics Committee of the Nordjylland Region (approval number N-20190036).

2.2. Experimental setup

The experimental paradigm follows from a previous experiment [22], which for the present study was extended across days. The methods are briefly described here. The experimental setup is shown in figure 1(C). Healthy participants wore an orthotic wrist immobilization splint to achieve near-isometric wrist flexion and extension movements. The Michelangelo prosthetic hand (OttoBock GmbH, DE) was attached to the splint, with the arm placed in the neutral position. Further, two dry EMG electrodes with embedded amplifiers (13E200, Otto Bock, DE) were placed over the wrist flexors and extensors of the right forearm. The electrode placement was determined by visually observing muscle contractions and palpating the forearm. In the case

of the individual with limb loss, the prosthesis was attached to a custom-made socket with integrated EMG electrodes. For all participants, five vibrotactors (C-2, Engineering Acoustics Inc.) were positioned evenly around a cross-section of the upper arm and secured in place by an elastic band. A modified box-and-blocks setup was used for the experimental task, where the participants were asked to apply predefined forces when grasping the blocks and to perform the task within a set time interval, as explained in the section ‘Experimental Design’. The prosthesis was connected to a standard laptop PC via Bluetooth, while the vibrotactors were connected via USB. The task instructions were displayed on a dedicated computer screen, positioned at a comfortable viewing angle and distance. The experiment was developed in MATLAB Simulink using a toolbox for testing human-in-the-loop control [27]. The control loop operated in real-time on the host PC at 100 Hz, through the Simulink Desktop Real-Time toolbox.

2.2.1. EMG control

All participants used near-isometric wrist flexion and proportional control to generate velocity commands to close the prosthesis. However, since fine control of prosthesis opening was not relevant to the study, it was simply triggered by a strong contraction of the wrist extensors. For the individual with limb loss, this meant that she was instructed to activate her residual wrist flexor and extensor muscles. The linear envelope of EMG was sampled at 100 Hz from two electrode systems, placed on the flexors and extensors, as explained above, through the

Table 1. The myoelectric command, prosthesis input and force ‘level’ boundaries for the discretized interface.

Level	0	1	2	3	4	5	6
Myoelectric command	0.025	0.1	0.27	0.47	0.69	0.95	1
Prosthesis input	0	0.25	0.42	0.59	0.76	0.9	1
Force	0.05	0.31	0.45	0.58	0.73	0.9	1

embedded prosthesis controller and transmitted to the host PC. The signals were subsequently filtered using a 2nd-order Butterworth low-pass filter with a 0.5 Hz cutoff, and this ‘myoelectric command’ from each of the electrodes was normalized to 50% of that obtained during maximum voluntary contraction (MVC) (following the results of [28]). The normalized myoelectric commands obtained from the flexor EMG were translated into the normalized input command for the prosthesis using a piecewise linear mapping defined by the breakpoints given in table 1 (see [22]). Note that the EMG intervals were wider for higher amplitudes to compensate for the higher variability of the EMG at stronger contractions. The prosthesis input command determined closing velocity (1—maximum velocity) and generated grasping force, i.e. the stronger the command input, the faster the prosthesis closes and the higher the force generated after contact. The aforementioned mapping effectively translated the EMG ‘levels’ into the corresponding force levels (see the next section for a more detailed explanation of closed-loop control). Note that for EMG amplitude lower than 0.025 on the normalized scale, no input command was sent to the prosthesis (Level 0) to avoid unintentional prosthesis closing. To trigger prosthetic hand opening, however, participants simply needed to reach 0.4 on the normalized range (i.e. 20% MVC) of extensor EMG.

2.2.2. Vibrotactile EMG feedback

All participants received feedback on self-generated flexor EMG command through a vibrotactor array. A spatial coding scheme consisting of six stimulation patterns was used to convey the six discrete levels of the myoelectric command. To represent the first five levels, one of the tactors from the array was activated individually in a specific order. However, the sixth level was indicated by activating all the tactors simultaneously (see figure 1(C)). During setup, adjustments were made to the position and/or intensity of the vibrotactors if they caused unpleasant or poorly localized sensations, to ensure that the participants could easily differentiate all the stimulation patterns. The vibration frequency for all tactors was set to 200 Hz, and the stimulation pattern was updated at 50 Hz.

The six discrete levels were defined using the same piece-wise linear mapping reported in table 1. As soon as the participants contracted their wrist flexors (to generate a myoelectric command above level 0), they received feedback about the level (1–6) they

were generating, thereby enabling them to modulate the prosthesis command input to the desired level using online feedback. The control and feedback interfaces were designed in such a way that if the participants generated a particular level of myoelectric command, the prosthesis applied the same level of force on the object. For instance, if a participant generated and maintained commands corresponding to level 2, the prosthesis closed at level 2 velocity and exerted level 2 force onto the grasped object. Note that while the feedback provided discrete information (a level of EMG), the command signal generated by the participant and transmitted to the prosthesis was still continuous and proportional (as in the commercial approach to prosthesis control). Therefore, if the EMG signal was in the higher range of level 2 (e.g. close to the threshold between levels 2 and 3), the generated grasping force would be in the higher range of level 2 of prosthesis forces, as defined by table 1.

2.3. Experimental design

The experiment was designed as a longitudinal trial over three sessions with a maximum of two days between the sessions. Here we describe the experimental design and protocol for the healthy participants first and point out the slight differences in the case study involving the individual with limb loss. In each session, the participants trained to perform the box-and-blocks task with the timed force-matching requirements. In each trial, they were required to (1) apply a specified level of force on the object (either level 3 or 5, see table 1), and (2) reach the target level within the specified time. Participants were required to perform the task in four speed conditions—Slow, Medium, Fast and Very Fast—which corresponded to time of execution in the range 4–8 s, 3–5 s, 2–4 s, and 1–3 s, respectively. The times of execution were defined to capture the relevant domains of the SAF curve and expand upon previous investigations [22]. Thereby, we used a time-band methodology to measure the SAF [20, 22] (i.e., to sample the shape of the SAF profile).

2.4. Experimental protocol

Initially, all equipment (the wrist immobilization splint (socket in the case of the individual with limb loss), prosthesis, EMG electrodes and vibrotactors) were placed on the participant. Then, a brief calibration and familiarization followed in all sessions. During EMG calibration, 3 repetitions of 5 s long MVC contractions were recorded independently for

both the flexors and extensors. The MVC measurements were recorded in the same posture that the participants would use to perform the box-and-blocks task, to account for the effect of arm posture and prosthesis weight on the recorded EMG. Next, the participants were guided to explore the control interface, i.e. the relation between muscle contraction intensity and velocity in hand opening/closing. Subsequently, they were familiarized with the vibrotactile feedback interface. This involved a spatial discrimination task where they were presented with two sets of 18 stimulation patterns (3 repetitions \times 6 levels, figure 1(C)) and asked to identify the patterns. The experiment proceeded once the participants achieved at least 95% success in the discrimination task, which usually required less than 5 min since the vibration patterns were designed to be easy to discriminate.

After familiarization with the control and feedback interfaces, participants performed 6 blocks of 32 trials (8 trials \times 4 speed conditions) of the timed force-matching task. On the first day, an extra (familiarization) block of 32 trials was performed where the participant was guided through the task. In each trial, the force and speed targets were first displayed. Then, the participants used the proportional control interface and the provided EMG feedback to successfully complete the trial, as explained in section 'Vibrotactile EMG feedback'. Once the participant felt they successfully reached (or overshoot) the target, they were instructed to trigger prosthesis opening. As the prosthesis was non-backdrivable, like most commercial devices, it was not possible to decrease the grasping force in a controlled manner (the prosthesis would open and release the object completely). Therefore, as explained before, the overshoot was also considered as a reason to open the hand and end the trial. Immediately after the trial ended, they received feedback on their performance, in terms of whether they acquired the target force and target speed. Such 'knowledge of results' has been shown to improve participants' motivation during the experiment and the rate of learning the task [29]. To some extent, this also reflects information that would be available in the daily use of a prosthesis (e.g. inappropriate force would lead to damaging or dropping of objects). However, the effect of this feedback is not explicitly addressed in this paper. During the familiarization trials, the participants were instructed on how to modulate their muscle contraction to control the closing velocity of the prosthesis. In each block of 32 trials, the target speed (Slow, Medium, Fast or Very Fast) was presented in a blocked fashion, i.e. it remained unchanged for 8 trials within which the target forces (3, 5) were presented 4 times each in random order. The target speeds were presented in a balanced random order, across blocks.

2.4.1. Experimental protocol for the individual with limb loss

The experimental protocol for the individual with a limb loss was slightly modified, where she performed 5 blocks (instead of 6) of trials with both force and speed targets on all three days. In addition, she performed 2 additional blocks of the same task but with no speed target (referred to as 'observational trials') on Day 2 and Day 3, to pilot test our model-based skill monitoring method. Given the additional blocks of observational trials on Days 2 and 3, we reduced the number of experimental blocks from 6 to 5 on all days, in the interest of not straining the participant. Apart from these modifications, the rest of the experiment proceeded identically to the healthy participants.

2.5. Outcome measures

During each trial, the recorded myoelectric commands and force measurements were processed to obtain the primary outcome measures—reach time and trial success, respectively. Reach time was calculated as the duration between the time when participant started generating the EMG input (above Level 0) and when the maximum force was reached during the trial. Therefore, a successful trial was defined as one where the reach time satisfied the speed requirement, and the maximum reached force was within the corresponding target force level. The trials were aggregated per speed condition to obtain percent success rates.

Further, to understand how the participants planned and executed the task across the sessions, we computed three behavioral metrics [22, 30]. We computed (1) the number of force corrections per trial that the participants made, by counting the number of distinct plateaus (longer than 250 ms) in the force trajectory [22], to gain insights into their control policies—specifically corresponding to how they included the supplementary feedback in their commands. Since EMG feedback promotes predictive modulation of commands, by allowing participants to adjust their muscle contraction during prosthesis closing so that the target force is generated at once, upon contact, without requiring further modulations [11, 25], the more successful the participants are in using this strategy, the lower the number of corrections. Further, we analyzed the quality of generated EMG commands, to understand if participants generated (2) smoother and (3) more repeatable EMG commands across days and speed targets. To evaluate smoothness, we calculated the spectral arc length (SPARC) of the EMG commands [31]. SPARC measures the negative arc length of the Fourier magnitude spectrum of the speed profile of a movement. Thereby, signals with a wider spectrum (and hence a

greater absolute SPARC value) are less smooth. We chose SPARC as an alternative to jerk-based measures, because it is a more general measurement of the smoothness of any movement-related variable and is robust to high-frequency changes in the recorded signal. To measure the repeatability of commands, we computed the trial-by-trial variability as follows: we first normalized all commands to 200 time points between the start of the trial and reach time, and then measured the standard deviation at each of the 200 time points. As the final measure of variability, we computed the median of the obtained standard deviations across the time points.

2.6. Parametric models of SAF

To capture the changes in the shape of the SAF curve across training (see figure 1(B)), we built a parametric model of SAF as $y = f(x; a, b)$, where y is success rate, x is reach time (duration of trial), and f is a function of x and two parameters a, b bearing functional forms already investigated in the literature. Specifically, we considered the power law equation described in [23, 26], relating the success rates and reach time developed in the context of 1-D cursor movements. While different in the functional form, the power law model is similar to (and simpler than) another model developed in the motor learning literature for a task that involved the production of a sequence of isometric finger forces [14]. Here we modified the equation to reflect the x -intercept (or asymptote) at 0.8 s, as it is impossible to get a successful trial below 0.8 s, due to limitations in the speed of the prosthesis response and EMG command generation:

$$y = 1 - a(x - 0.8)^b. \quad (1)$$

Note that parameter b in equation (1) is restricted to be negative.

2.6.1. Model fitting

The models were fit for day-wise pooled healthy participants' data (success rate and reach time) for each of the 3 days, using ordinary least squares-based fitting. Success rates and reach times from 2 consecutive blocks were averaged so that the mean success rate and its variance are well represented during model fitting. This way, the power-law model was fitted using 12 points (4 speeds \times 3 points per speed). The parameters obtained through this fitting procedure are denoted by asterisks, such as (a^*, b^*) . The goodness of fit was measured using the R^2 metric.

All models were log-transformed before fitting so that the parameters obtained would be easy to interpret. This way, parameter 'log a ' denotes the y -intercept of the SAF in the log-log plane, while 'b' denotes the slope at which the success rate increases with reach time. A change (exclusively) in the intercept therefore indicates that the log-success rates at

all movement speeds are affected similarly (e.g. consistent increase at all speeds), while a change in slope indicates that different speeds may affect success rate differently (e.g. increase at low speeds and decrease for high speeds).

2.6.2. Reducing model complexity: from 2-parameter to 1-parameter models

Earlier studies have observed that the SAF models described above can be further simplified such that only a single parameter reflects skill-related changes [14, 23], but as explained before, this has been established for motor control tasks involving natural movements. Here, in a similar vein, we investigated if one parameter reflected skill improvements while the other parameter could be fixed in the context of closed-loop prosthesis control. In other words, we were interested in finding if $f(x; a, b) \approx f(x; a, \underline{b})$ or $f(x; a, b) \approx f(x; \underline{a}, b)$, where the underscore denotes the parameter being held constant. To start, let us denote the R^2 obtained by fitting a particular set of data $\{y, x\}_i$ to the 2-parameter model such that $R_i^2(a^*, b^*) := R^2(y_i, f(x_i; a^*, b^*))$, where $i = \{1, 2, 3\}$ denotes the pooled success rate (y_i) and reach time (x_i) dataset of a particular day and a^*, b^* , denote the best-fit parameters.

Then, ΔR^2 represents the change in the goodness of fit (R^2) when using the 1-parameter model, e.g. obtained by fixing a constant at a^* and setting b to b_k in the vicinity of b^* . A significant decrease in R^2 due to such a perturbation in one of the parameters (a or b) indicates that perturbing that parameter leads to worse fits with respect to the full 2-parameter model. By quantifying the sensitivity of the model fits to both parameters, we can rigorously quantify how they affect the goodness of fit and choose which parameter to set as a constant. Accordingly, we selected 1000 values of a and b in the range of the parameters in the vicinity of those observed by fitting the experimental data, (a_{\min}, a_{\max}) and (b_{\min}, b_{\max}) and computed the following set of R^2 values:

$$\Delta R^2(a_j) := \{R_i^2(a_j, b^*) - R_i^2(a^*, b^*), \forall i\}, \\ a_j \in (a_{\min}, a_{\max}),$$

$$\Delta R^2(b_k) := \{R_i^2(a^*, b_k) - R_i^2(a^*, b^*), \forall i\}, \\ b_k \in (b_{\min}, b_{\max}),$$

where index $i = \{1, 2, 3\}$ denotes the *day*. We then obtain the simplified 1-parameter model by finding the parameter that changed mean R^2 the least,

$$\bar{a} = \arg \min_a \langle \Delta R^2(a_j) \rangle, \text{ or } \bar{b} = \arg \min_b \langle \Delta R^2(b_k) \rangle$$

where $\langle \cdot \rangle$ denotes the mean of the set of values ΔR^2 .

2.7. Statistical analysis

3-factor repeated measures ANOVAs for success rate and behavioral measures were fit with 3 within-subjects factors—day, target speed and target force. To analyze the total improvement between Day 1 and 3, we fit 2-factor ANOVAs with target force and target speed as the factors. The assumptions of normality, homogeneity of variance and sphericity were verified using Shapiro-Wilk's, Levene's and Mauchly's tests, respectively. Post-hoc analyses for all quantities of interest were performed by using pairwise t -tests, adjusted using the Holm–Bonferroni method. The threshold for statistical significance was set at $p < 0.05$. The mean \pm standard deviation of outcomes per group of interest are reported throughout the paper.

3. Results

3.1. Learning induced changes in the SAF

We analyzed how participants' SAFs (see figure 2(A)) changed across the experiment by fitting a 3-way ANOVA with day, target speed and target force as factors. We found that all three factors significantly influenced the success rate (day: $F(2, 30) = 14.05$, $p = 5 \times 10^{-5}$, target speed: $F(3, 45) = 35.47$, $p = 6 \times 10^{-12}$, and target force: $F(1, 15) = 9.46$, $p = 7 \times 10^{-3}$), but none of the factor interactions was significant. Participants exhibited a wide range of success rates across days and speeds, ranging from $66.3 \pm 15.2\%$ in the Very Fast speed on Day 1, to $90.2 \pm 10\%$ in the Slow speed on Day 3. Post-hoc analyses revealed that success rates improved significantly from Day 1–2 ($p\text{-adj} = 0.01$), and Day 1–3 ($p\text{-adj} = 0.0008$) while the difference from Day 2–3 was not significant (Day 1: $75.4 \pm 14.6\%$, Day 2: $81.7 \pm 13.3\%$, and Day 3: $85.3 \pm 10.8\%$; average success rates across speeds). In a similar way, the participants' success rates significantly increased from Very Fast to Fast ($p\text{-adj} = 0.005$) and Fast to Medium ($p\text{-adj} = 7 \times 10^{-4}$) but not from Medium to Slow speed. A significant effect of target force meant that participants were more successful in target Level 5 than Level 3 throughout (Level 3: $77.8 \pm 14.4\%$, Level 5: $83.8 \pm 12.1\%$; averaged across speeds and days, figure 2(A), right).

Next, we analyzed how SAF changed between Day 1 and Day 3. Interestingly, while participants' success rates improved across days, as explained above, there was no significant effect of target speed or target force on the observed improvement. That is, the increase in the success rate was similar across speeds though with large variability (Very Fast: $12.7 \pm 15.6\%$, Fast: $7.6 \pm 12.9\%$, Medium $9.8 \pm 7.7\%$, and Slow $7.1 \pm 9.7\%$, averaged across force levels, see figure 2(B)), and across force levels (Level 3: $9.8 \pm 8.8\%$, Level 5: $8.8 \pm 8.7\%$, averaged across speeds). Therefore, the SAF curve effectively 'shifted upwards' across days consistently for all speeds, at both force levels.

Results of the individual with a limb loss largely followed the trends of the healthy participants, however, her success rate improved only slightly from 84.8% on Day 1 to 86.3% on Day 3 (stars in figures 2(A) and (B)).

3.2. Behavioral analyses

We then analyzed how participants' behavior (planning and execution of EMG commands) changed across days. First, we investigated how participants' control policies changed with training, by looking at the number of force corrections generated (figure 2(C)), the number of corrections are averaged over the two target forces to emphasize the effect of training (changes across days)). We found that the control policies were affected by the target speed ($F(3, 45) = 634.0$, $p < 1 \times 10^{-10}$), and target force ($F(1, 15) = 843.7$, $p < 1 \times 10^{-10}$). However, there was no significant effect of day, indicating that the overall strategy of how participants used the feedback remained consistent throughout the experiment. There was an interaction effect between target force and speed ($F(3, 45) = 115.8$, $p < 1 \times 10^{-10}$), whereby the number of corrections for target level 3 decreased more gradually with speed, compared to level 5. The number of corrections decreased steadily with the target speed (post-hoc tests were significant for all pairs, with each $p\text{-adj} < 1 \times 10^{-7}$), suggesting that at faster speeds, participants adjusted their muscle contractions prior to contacting the object, rather than using feedback post-contact to reach the required force. Finally, participants made fewer corrections to reach force level 3 than level 5 ($p < 1 \times 10^{-10}$).

Next, we analyzed how the smoothness and trial-by-trial variability of their movements were influenced by learning (figures 2(D) and (E)), both measures are shown by averaging across target force levels, similar to figure 2(C)). We found that there was a significant effect of all three independent variables—target speed, target force and day on both metrics (see table 2). Additionally, there was a significant interaction effect of target speed and target force on movement smoothness ($F(3, 45) = 69.8$, $p < 1 \times 10^{-10}$), such that the smoothness of commands to reach target level 3 decreased more rapidly with speed, compared to level 5. Surprisingly, smoothness decreased from Day 1–3 ($p\text{-adj} = 6 \times 10^{-4}$), without any significant changes on consecutive days, while the smoothest trajectories were observed at the fastest speeds (post-hoc tests were significant for all pairs, with each $p\text{-adj} < 1 \times 10^{-8}$). On the other hand, variability decreased from Day 1–2 ($p\text{-adj} = 0.002$) and then stagnated. Moreover, it was significantly different between the faster and slower speeds, with a significant difference between Fast and Medium ($p\text{-adj} = 0.046$), but not between Fast and Very Fast or Medium and Slow. Finally, while participants produced smoother commands to reach force

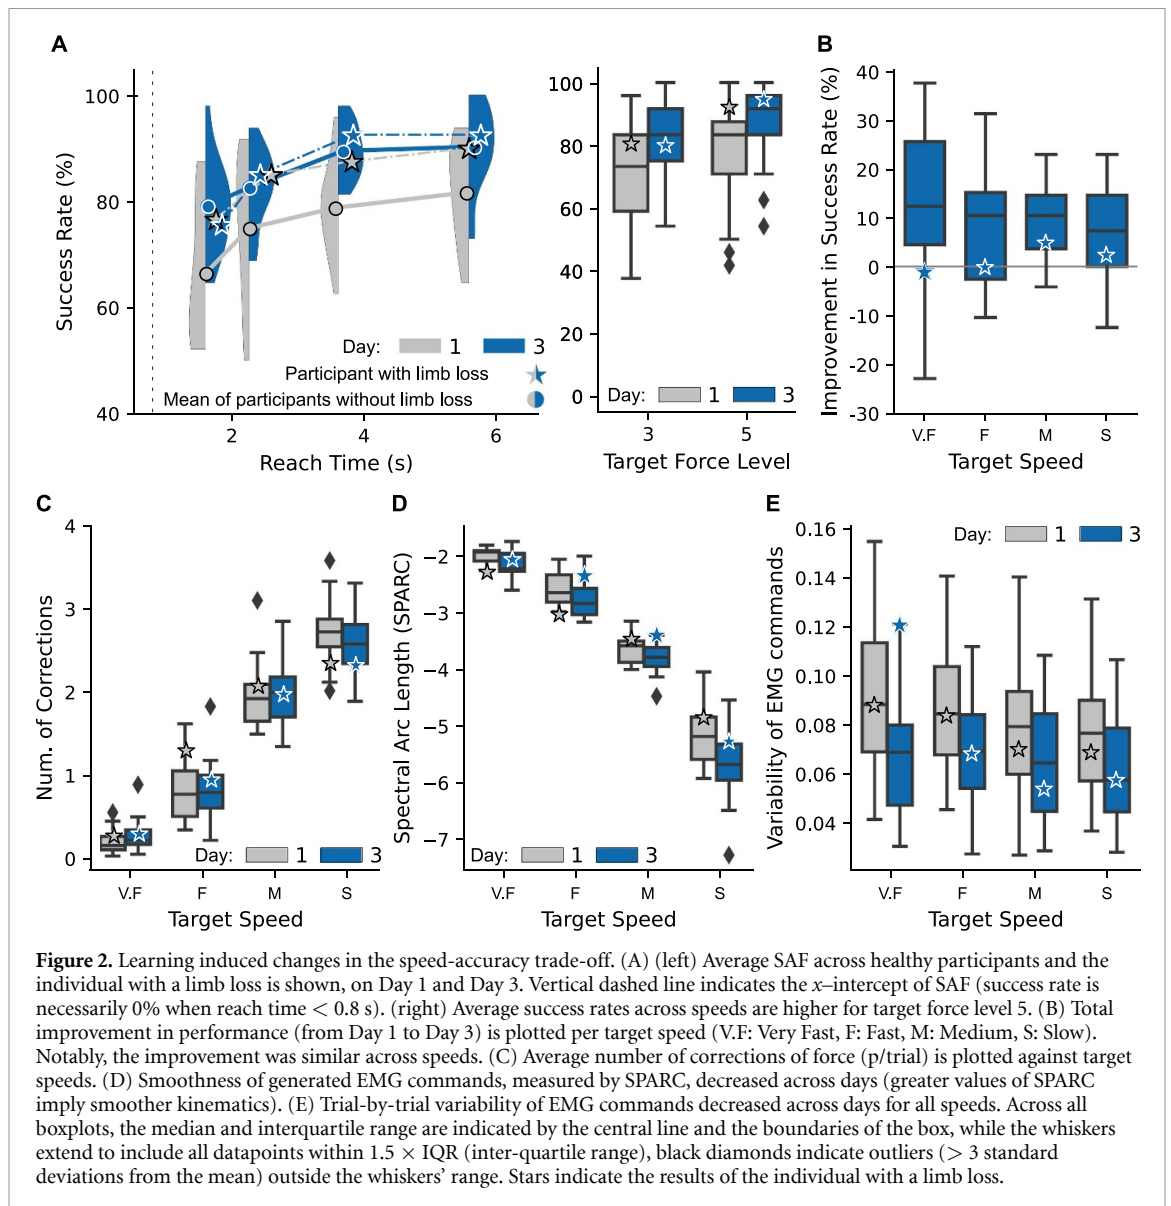


Figure 2. Learning induced changes in the speed-accuracy trade-off. (A) (left) Average SAF across healthy participants and the individual with a limb loss is shown, on Day 1 and Day 3. Vertical dashed line indicates the x -intercept of SAF (success rate is necessarily 0% when reach time < 0.8 s). (right) Average success rates across speeds are higher for target force level 5. (B) Total improvement in performance (from Day 1 to Day 3) is plotted per target speed (V.F: Very Fast, F: Fast, M: Medium, S: Slow). Notably, the improvement was similar across speeds. (C) Average number of corrections of force (p/trial) is plotted against target speeds. (D) Smoothness of generated EMG commands, measured by SPARC, decreased across days (greater values of SPARC imply smoother kinematics). (E) Trial-by-trial variability of EMG commands decreased across days for all speeds. Across all boxplots, the median and interquartile range are indicated by the central line and the boundaries of the box, while the whiskers extend to include all datapoints within $1.5 \times \text{IQR}$ (inter-quartile range), black diamonds indicate outliers (> 3 standard deviations from the mean) outside the whiskers' range. Stars indicate the results of the individual with a limb loss.

Table 2. Main effects of target speed, target force and day on the behavioral metrics considered in the study, obtained using a 3-way ANOVA (see Methods).


	Target speed	Target force	Day
Number of corrections	$F(3, 45) = 634.0, p < 1 \times 10^{-10}$	$F(1, 15) = 843.7, p < 1 \times 10^{-10}$	$F(2, 30) = 0.08, p = 0.92$
Smoothness	$F(3, 45) = 373.8, p < 1 \times 10^{-10}$	$F(1, 15) = 79.8, p = 2 \times 10^{-7}$	$F(2, 30) = 7.7, p = 0.002$
Trial-by-trial variability	$F(3, 45) = 10.1, p = 3 \times 10^{-5}$	$F(1, 15) = 128.9, p = 9 \times 10^{-9}$	$F(2, 30) = 19.2, p = 4 \times 10^{-6}$

level 5 (compared to level 3 $p = 2 \times 10^{-6}$), the variability of those commands was significantly larger than while reaching level 3 ($p = 9 \times 10^{-9}$). Behavioral results of the participant with limb loss also largely mirrored her healthy counterparts, except for movement smoothness which improved across days (figures 2(C)–(E)).

3.3. Skill monitoring using ‘observational’ trials and SAF models

A power-law model of SAF with 2 parameters was fit to log-transformed performance data obtained by

pooling across participants (see section 2.6). Across the three days, the average R^2 was 0.76 ± 0.09 . Figure 3(A) displays the model fit in the log-log plane (and figure 3(B) in true coordinates) where the data was pooled across subjects and demonstrates that the slope of the SAF remained similar across training (Day 1–3: $-0.49, -0.57, -0.58$), while the intercept decreased (Day 1–3: $-1.18, -1.42, -1.63$), which is in line with the conclusions of previous studies [14, 23]. Therefore, we proceeded to simplify the 2-parameter model by fixing the slope. To determine the parameter value of the slope that least affected the

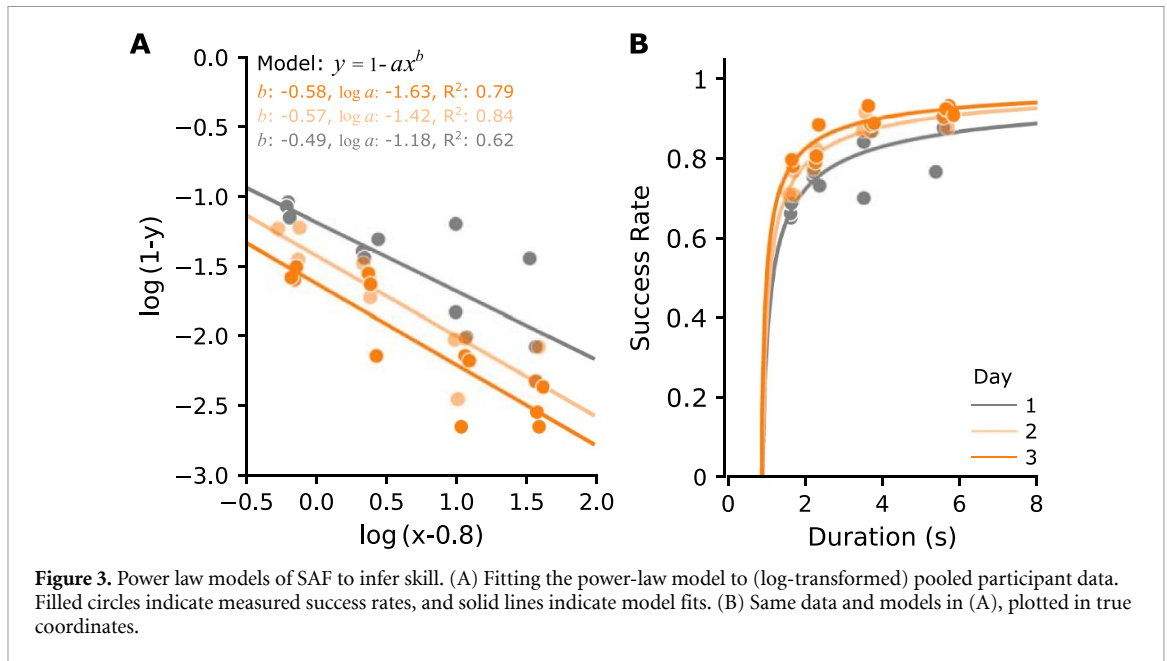

R^2 of the model fits across the three days, we conducted a perturbation analysis where we fixed the intercept to its true value and varied the slope in the vicinity of the best-fit values obtained above. We found that when the slope was fixed at -0.55 , we observed almost no loss in the goodness of fit across the three days (a decrease of 0.009 in R^2). In comparison, fixing the intercept led to a decrease of at least 0.18 in R^2 . Therefore, we fixed the slope to be -0.55 for our 1-parameter model.

Using this 1-parameter model, we proceeded to infer skill changes in the case study involving an individual with limb loss. During the SAF trials, the participant's success rate slightly improved (2.6% increase, averaged across speeds) from Day 1 to Day 3, which together with the improved trial-by-trial variability indicates a slight improvement in skill. Apart from the SAF experiment, where execution speed was controlled, the participant also performed 'observational' trials where the speed was unrestricted, on Day 2 and Day 3. During these trials, the average success rate increased from $89.1 \pm 9.2\%$ to $96.8 \pm 3.1\%$, but with an accompanied increase in reach times (decreased speed) from 1.95 ± 0.3 s to 2.96 ± 0.27 s, thereby making skill inference infeasible using just success rate and reach time data. We subsequently fit the 1-parameter SAF model, to analyze if there is a change in the intercept. We found that there is a decrease in the intercept from -2.14 to -3.02 , indicating a trend towards improvement of skill. While the intercept values obtained were larger than those for the pooled healthy-participant data, this can be explained by the difference in average performance between the pooled participant (speed-restricted) trials and the observational trials of the individual with limb loss.

4. Discussion

SAFs provide a rigorous way to evaluate and understand motor skill and monitor its improvement across days. Here, we empirically measured how the SAF changed across three days for a prosthesis force control task where participants used a closed-loop interface based on proportional myoelectric control and EMG feedback. We found that the shape of the SAF curve remained intact, as participants' success rate improved similarly across all speeds and forces. We then built parametric models of the measured SAFs to better characterize the changes in SAF and discussed a method to monitor skill changes using observational data from an individual with a limb loss.

4.1. Learning induced changes in the SAF for an EMG feedback-based interface

In this study, we focused on an EMG feedback-based interface that has previously been shown to outperform other non-invasive feedback approaches to prosthesis force control [25, 32]. We elicited a wide range of success rates by enforcing task execution at different speeds using a time-band methodology, similar to previous studies that investigated motor control of natural movements [16, 22]. We found a significant improvement in performance with training across all speeds. We expected that the largest gains in the SAF would occur toward faster speeds (Fast and Very Fast), due to the nature of EMG feedback which promotes predictive modulation of muscle contractions [11, 24]. However, conversely, we found that the SAF merely 'shifted upwards'. Nevertheless, the shape of the SAF curve flattened at slower speeds (no difference between Medium and

Slow), and it would be interesting to analyze whether prolonged training would eventually change the profile shape by flattening out the other side of the curve (i.e. similar performance across all speeds).

We also noticed that the shape of the SAF was similar across force targets. Interestingly, we found that the participants had greater success reaching target level 5 compared to 3, even at faster speeds. This could be attributed to the design of our piece-wise linear control mapping, which ensures that the variability at stronger contractions is compensated for by the width of the levels. In addition, most of the improvement happened quickly, after a single day of training (from Day 1 to Day 2). It remains to be tested if the lack of significant improvement between Days 2 and 3 means that this is the maximum performance or, more likely, that prolonged training would lead to further improvement but with more gradual increments. Taken together, these outcomes are encouraging for the application of EMG feedback, demonstrating that it affords a consistent and steady improvement in skill over a range of speeds and forces.

Underlying these changes in performance, we observed that the behavioral outcome measures also exhibited interesting trends during training. First, there was no change, across days, in the strategy adopted by participants in each of the speed conditions, as shown by the number of corrections they used to achieve the target force. This indicates that training across days primarily affected participants' motor execution. At the level of generated EMG commands, we observed that the signals became less variable (or more similar to each other from trial to trial) across days, indicating that participants' motor execution became more stereotypical, a hallmark of skilled behavior. However, counterintuitively, the commands also became less smooth. This could be due to the discretized nature of the task and feedback interface, which promotes participants to navigate from one level to the next, by 'pausing' in between to avoid overshooting, and thereby leading to less smooth trajectories as participants pause for shorter periods of time. In essence, this ability to exploit a 'pausing'-based strategy enabled by the interface reflects an improved skill to fine-tune EMG commands and thereby navigate the force levels more reliably. It is important to note that this decrease in smoothness, together with the number of force corrections, is caused by the discretized interface at hand and therefore these metrics might behave differently, e.g. for an interface with continuous feedback such as through amplitude modulation of a single vibrotactor. Overall, we demonstrated the utility of measuring motor execution related metrics to understand how kinematic and user-generated variables could be employed to understand how different interfaces enable users to acquire skilled behavior. Naturally, this can be extended to different tasks, for

instance, grasping of a compliant object that would enable force adjustments in both directions as well as strengthen the incidental feedback (e.g. force estimated from object deformation). An interesting direction of future research could be to investigate how motor execution changes in such a situation.

Notably, the performance and behavioral outcomes of the participant with limb loss largely mirrored that of her healthy counterparts. However, the amount of improvement she showcased was much less compared to the healthy participants, partly explained by her previous experience with myoelectric control and EMG feedback as well as prosthesis use in daily life. Despite the lack of a significant improvement in success rate, both movement smoothness and variability improved at three out of four speeds. This underscores the relevance of measuring movement characteristics to better monitor user skill progression, as has also been highlighted in earlier studies [8, 9]. Moreover, it substantiates the utility of analyzing trial-by-trial variability of myoelectric commands as a marker of skill, analogous to reduced variability of end-point kinematics in natural movements [17, 18].

4.2. Measuring and monitoring skill through SAF models

Speed and accuracy of movements are inextricably linked, and skill can be best understood as a combination of the two. SAFs therefore provide a quantitative framework through which to measure skill. In combination with previous results where SAF was introduced as a means of comparing and evaluating different closed-loop prosthesis interfaces (Force vs. EMG feedback) [22], here we observed that the SAFs so measured do not change shape across days, at least for the EMG feedback interface. The constancy of tradeoff (here observed with respect to both force levels and speeds) might be a more general phenomenon [16], as also reflected in studies of the intact motor system. This raises an interesting possibility—given that participants improve similarly across speeds, the tradeoff enabled by one interface may be different than another no matter the level of training of the user. For example, in [27], the benefits of EMG feedback with respect to force feedback were most expressed for medium speeds, and the present study implies that this might persist regardless of training. However, this still needs to be confirmed experimentally.

Additionally, here we encapsulated the SAFs using a power law model, whereby the parameters of the model completely determined the SAF. Accordingly, empirically estimating the model parameters and investigating how they change over time gives us a powerful methodology to measure and monitor user skill progression. In line with previous efforts [14, 23], we observed that the exponent of the power law model (slope in log-transformed coordinates)

remained relatively constant. We leveraged this knowledge to overcome one potential limitation of the SAF methodology—that participants need to repeat the same task at multiple speeds, requiring more experimental time than the common practice of performing the task at a single self-chosen speed. However, given the narrow variability in the observational data, it remains to be seen if a single execution speed sufficiently estimates the parameter of interest or if experimentally sampling more speeds might lead to better estimates. Due to this and other limitations outlined in the next section, the presented analysis and application of a single-parameter model shall be regarded as a proof-of-concept. Furthermore, while such a simplified SAF model perhaps enables skill inference and provides a good approximation of the SAF, we believe that measuring the SAF and the underlying motor execution, is substantially more informative.

4.3. Limitations and future work

One limitation of the current study is the inclusion of only a single individual with limb loss. However, considering the alignment of performance and behavioral metrics of the individual with limb loss and the healthy cohort in this study, coupled with the simplicity of the interface and task used, we expect that the results are likely to translate to individuals with limb loss, even more so to those with less experience in prosthesis control. Nevertheless, tests in a larger pool of amputees are the necessary next step in this research. Another important limitation is that we only conducted the observational experiment on the individual with limb loss. Moreover, we observed that she had very high levels of skill, already to begin with, having participated in similar experimental setups before, and therefore did not improve by much. Therefore, future studies need to verify the validity of the proposed model-based skill inference framework with a larger cohort of participants with measured SAF profiles in combination with observational data. However, we believe that the approach of modelling SAFs and incorporating that knowledge to infer skill represents a promising direction to promote rigorous skill inference, and for benchmarking efforts that characterize the performance afforded by different interfaces. The latter can also include the baseline condition, with no artificial sensory feedback, where prosthesis users can only rely on incidental sources of information (visual and auditory cues). This would allow quantifying the state of the art in ‘open-loop’ user-prosthesis interfaces as well as reveal the benefits of added feedback.

5. Conclusion

In this study, we empirically derived the changes in SAFs during a three day experiment, as participants performed a functional prosthesis force-matching task. We found that success rates increased from Day

1 to Day 3, and that the improvement was similar across the target forces and target speeds. The training therefore improved performance without altering the initial shape of the SAF profile. We then modeled the empirically observed profiles to thoroughly characterize learning induced changes in SAF with EMG feedback. More generally, the study demonstrates that the SAF methodology can be successfully translated to prosthesis control for systematic and comprehensive monitoring of user skill.

Data availability statement

The data cannot be made publicly available upon publication due to legal restrictions preventing unrestricted public distribution. The data that support the findings of this study are available upon reasonable request from the authors.

Acknowledgments

This work has been supported by the Projects 8022-00243A (ROBIN) and 8022-00226B funded by the Independent Research Fund Denmark. We thank Jacob Nebeling Hedegaard for helpful discussions regarding SAF model fitting and comparison.

ORCID iDs

Pranav Mamidanna  <https://orcid.org/0000-0002-2095-3314>

Dario Farina  <https://orcid.org/0000-0002-7883-2697>

Jakob Lund Dideriksen  <https://orcid.org/0000-0001-6587-0865>

Strahinja Dosen  <https://orcid.org/0000-0003-3035-147X>

References

- [1] Farina D *et al* 2021 Toward higher-performance bionic limbs for wider clinical use *Nat. Biomed. Eng.* **7** 473–85
- [2] Bensmaïa S J, Tyler D J and Micera S 2020 Restoration of sensory information via bionic hands *Nat. Biomed. Eng.* **7** 1–13
- [3] Pasluosta C, Kiele P, Čvančara P, Micera S, Aszmann O C and Stieglitz T 2022 Bidirectional bionic limbs: a perspective bridging technology and physiology *J. Neural Eng.* **19** 013001
- [4] Schofield J S, Shell C E, Beckler D T, Thumser Z C and Marasco P D 2020 Long-term home-use of sensory-motor-integrated bidirectional bionic prosthetic arms promotes functional, perceptual, and cognitive changes *Front. Neurosci.* **14** 120
- [5] Osborn L E *et al* 2021 Extended home use of an advanced osseointegrated prosthetic arm improves function, performance, and control efficiency *J. Neural Eng.* **18** 026020
- [6] Butkus J Upper extremity prosthetic rehabilitation: a 20 day plan of therapy, education and coaching *Myoelectric Controls and Upper Limb Prosthetics Symp.* pp 14–16
- [7] Salminger S *et al* 2020 Current rates of prosthetic usage in upper-limb amputees—have innovations had an impact on device acceptance? *Disabil. Rehabil.* **44** 1–12

- [8] Bouwsema H, Kyberd P J, Hill W, van der Sluis C K and Bongers R M 2012 Determining skill level in myoelectric prosthesis use with multiple outcome measures *J. Rehabil. Res. Dev.* **49** 1331–47
- [9] Bouwsema H, van der Sluis C K and Bongers R M 2014 Changes in performance over time while learning to use a myoelectric prosthesis *J. Neuroeng. Rehabil.* **11** 16
- [10] Sensinger J W and Dosen S 2020 A review of sensory feedback in upper-limb prostheses from the perspective of human motor control *Front. Neurosci.* **14** 345
- [11] Strbac M, Isakovic M, Belic M, Popovic I, Simanic I, Farina D, Keller T and Dosen S 2017 Short- and long-term learning of feedforward control of a myoelectric prosthesis with sensory feedback by amputees *IEEE Trans. Neural Syst. Rehabil. Eng.* **25** 2133–45
- [12] van Dijkvan Dijk L, van der Sluis C K, van Dijkvan Dijk H W and Bongers R M 2016 Learning an EMG controlled game: task-specific adaptations and transfer *PLoS One* **11** e0160817
- [13] Kristoffersen M B, Franzke A W, van der Sluis C K, Murgia A and Bongers R M 2019 The effect of feedback during training sessions on learning pattern-recognition-based prosthesis control *IEEE Trans. Neural Syst. Rehabil. Eng.* **27** 2087–96
- [14] Reis J, Schambra H M, Cohen L G, Buch E R, Fritsch B, Zarahn E, Celnik P A and Krakauer J W 2009 Noninvasive cortical stimulation enhances motor skill acquisition over multiple days through an effect on consolidation *Proc. Natl Acad. Sci.* **106** 1590–5
- [15] Dayan E and Cohen L G 2011 Neuroplasticity subserving motor skill learning *Neuron* **72** 443–54
- [16] Shmuelof L, Krakauer J W and Mazzoni P 2012 How is a motor skill learned? Change and invariance at the levels of task success and trajectory control *J. Neurophysiol.* **108** 578–94
- [17] Krakauer J W, Hadjiosif A M, Xu J, Wong A L and Haith A M 2019 Motor learning *Comprehensive Physiology* 1st edn, ed R Terjung (Wiley) pp 613–63
- [18] Sternad D 2018 It's not (only) the mean that matters: variability, noise and exploration in skill learning *Curr. Opin. Behav. Sci.* **20** 183–95
- [19] Shmuelof L, Yang J, Caffo B, Mazzoni P and Krakauer J W 2014 The neural correlates of learned motor acuity *J. Neurophysiol.* **112** 971–80
- [20] Wickelgren W A 1977 Speed-accuracy tradeoff and information processing dynamics *Acta Psychol.* **41** 67–85
- [21] Heitz R P 2014 The speed-accuracy tradeoff: history, physiology, methodology, and behavior *Front. Neurosci.* **8** 150
- [22] Mamidanna P, Dideriksen J L and Dosen S 2022 Estimating speed-accuracy trade-offs to evaluate and understand closed-loop prosthesis interfaces *J. Neural Eng.* **19** 056012
- [23] Guiard Y, Olafsdottir H B and Perrault S T 2011 Fitt's law as an explicit time/error trade-off *Proc. SIGCHI Conf. on Human Factors in Computing Systems (ACM)* pp 1619–28
- [24] Dosen S, Markovic M, Somer K, Graimann B and Farina D 2015 EMG Biofeedback for online predictive control of grasping force in a myoelectric prosthesis *J. Neuroeng. Rehabil.* **12** 55
- [25] Schweisfurth M A, Markovic M, Dosen S, Teich F, Graimann B and Farina D 2016 Electrotactile EMG feedback improves the control of prosthesis grasping force *J. Neural Eng.* **13** 056010
- [26] Guiard Y and Rioul O 2015 A mathematical description of the speed/accuracy trade-off of aimed movement *Proc. 2015 British HCI Conf. (ACM)* pp 91–100
- [27] Dosen S, Markovic M, Hartmann C and Farina D 2015 Sensory feedback in prosthetics: a standardized test bench for closed-loop control *IEEE Trans. Neural Syst. Rehabil. Eng.* **23** 267–76
- [28] Tchिमino J, Markovic M, Dideriksen J L and Dosen S 2021 The effect of calibration parameters on the control of a myoelectric hand prosthesis using EMG feedback *J. Neural Eng.* **18** 046091
- [29] Sigrist R, Rauter G, Riener R and Wolf P 2013 Augmented visual, auditory, haptic, and multimodal feedback in motor learning: a review *Psychon. Bull. Rev.* **20** 21–53
- [30] Mamidanna P, Dideriksen J L and Dosen S 2021 The impact of objective functions on control policies in closed-loop control of grasping force with a myoelectric prosthesis *J. Neural Eng.* **18** 056036
- [31] Balasubramanian S, Melendez-Calderon A, Roby-Brami A and Burdet E 2015 On the analysis of movement smoothness *J. Neuroeng. Rehabil.* **12** 112
- [32] Tchिमino J, Dideriksen J L and Dosen S 2022 EMG feedback outperforms force feedback in the presence of prosthesis control disturbance *Front. Neurosci.* **16** 952288