



**AALBORG UNIVERSITY**  
DENMARK

**Aalborg Universitet**

## **Improved PID control for triaxial testing liquefied specimen**

Sabaliauskas, Tomas; Ibsen, Lars Bo

*Publication date:*  
2017

*Document Version*  
Publisher's PDF, also known as Version of record

[Link to publication from Aalborg University](#)

*Citation for published version (APA):*  
Sabaliauskas, T., & Ibsen, L. B. (2017). *Improved PID control for triaxial testing liquefied specimen*. Department of Civil Engineering, Aalborg University. DCE Technical reports No. 232

### **General rights**

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal -

### **Take down policy**

If you believe that this document breaches copyright please contact us at [vbn@aub.aau.dk](mailto:vbn@aub.aau.dk) providing details, and we will remove access to the work immediately and investigate your claim.



**DEPARTMENT OF CIVIL ENGINEERING**  
AALBORG UNIVERSITY

# **Improved PID control for triaxial testing liquefied specimen**

**Tomas Sabaliauskas  
Lars Bo Ibsen**



Aalborg University  
Department of Civil Engineering  
Group Name

**DCE Technical Report No. 232**

# **Improved PID control for triaxial testing liquefied specimen**

by

Tomas Sabaliauskas  
Lars Bo Ibsen

October 2017

© Aalborg University

## Scientific Publications at the Department of Civil Engineering

**Technical Reports** are published for timely dissemination of research results and scientific work carried out at the Department of Civil Engineering (DCE) at Aalborg University. This medium allows publication of more detailed explanations and results than typically allowed in scientific journals.

**Technical Memoranda** are produced to enable the preliminary dissemination of scientific work by the personnel of the DCE where such release is deemed to be appropriate. Documents of this kind may be incomplete or temporary versions of papers—or part of continuing work. This should be kept in mind when references are given to publications of this kind.

**Contract Reports** are produced to report scientific work carried out under contract. Publications of this kind contain confidential matter and are reserved for the sponsors and the DCE. Therefore, Contract Reports are generally not available for public circulation.

**Lecture Notes** contain material produced by the lecturers at the DCE for educational purposes. This may be scientific notes, lecture books, example problems or manuals for laboratory work, or computer programs developed at the DCE.

**Theses** are monographs or collections of papers published to report the scientific work carried out at the DCE to obtain a degree as either PhD or Doctor of Technology. The thesis is publicly available after the defence of the degree.

**Latest News** is published to enable rapid communication of information about scientific work carried out at the DCE. This includes the status of research projects, developments in the laboratories, information about collaborative work and recent research results.

Published 2017 by  
Aalborg University  
Department of Civil Engineering  
Thomas Manns vej 23, 9200  
Aalborg, Denmark

Printed in Aalborg at Aalborg University

ISSN 1901-726X  
DCE Technical Report No. 232

# Improved PID control for triaxial testing liquefied specimen

Tomas Sabaliauskas, Lars Bo Ibsen.

## ABSTRACT

Using a frictionless triaxial apparatus, sand specimens can be tested at relatively high axial strains, even while liquefying. However, liquefying specimens have extremely nonlinear stiffness, thus standard PID control does not perform well. To maintain control over applied loads, the PID controller was modified to adapt to disturbed soil states.

The proposed methods expand the scope of testing towards options which are otherwise inaccessible by triaxial testing.

## INTRODUCTION

A single diameter height specimen tested using frictionless triaxial apparatus is very durable. It can be compressed beyond yielding and pulled back to initial length – both drained and undrained. Such specimens yield isotropically, without forming a dominant shear rupture (in contrast to conventional triaxial apparatus). If no water is added, unsaturated specimens can develop multiple failure planes simultaneously (Fig. 1). Whereas saturated specimens – do not form shear rupture at all when compressed.

Due to isotropic strain (and stress) distribution, specimen durability increases dramatically. A fully saturated sample can be crushed beyond 10% axial strain without forming a shear band or bulging. And the deformation remains reversible, the sample can be pulled back to initial length, liquefied, drained and repeatedly cyclic tested in one, long, aggressive sequence. A sample liquefied and drained 6 times is shown in Fig. 2. The extreme scope of testing is obtained using two factors. First – mechanical properties of the frictionless apparatus, which preserves the specimen shape and durability. Second – load control methods, which adapt to changing specimen stiffness and strength, thus ensuring the end plates will stay in contact with the specimen being tested.

Triaxial apparatus is rather simple in construction. At the bottom a piston moves up and down, moving the bottom end plate with it. At the top, an end plate is fixed to a load cell (Ibsen, L. B., 1995). A proportional integral distance (PID) controller can

move the bottom piston to a user defined target position (U) or force (F), where F is measured by the load cell. Thus, a PID controlled can operate either in displacement mode or force mode (U or F mode).

In standard tests target U or target F can be specified manually, or set to follow a pre-defined wave shape (sinusoidal, saw tooth, square wave, etc.). These options are available by default in the software used to control the (dynamic) Danish triaxial apparatus. Each wave shape has unique benefits and limitations.

### Linear ramp loading

The most basic type of loading is linear ramp. The load is applied at a constant rate, either  $\Delta F/\Delta t$  or  $\Delta U/\Delta t$ , towards the target F or U. Cyclic loading tests start with linear ramp "preloading" towards the average Force ( $F_a$ ). A linear loading path can be seen going towards  $F_a$  in Figs. 3-6. The produced loading path looks like a line, but the PID controller is adjusting piston position a thousand times per second – to keep the real time value of F or U "on target".

One must recognize that the PID controller is predicting how many "injections of oil" need to be supplied to the piston, in effort to keep the measured F (or U) "on target". The number of injections is calibrated by three coefficients – P, I and D. The coefficients are found through trial and error and as long as F (or U) response remains somewhat linear the PID calibration performs well. The PID controller works especially well with U control. Hydraulic fluid is extremely stiff, thus the same number of oil injections will produce the same amount of displacement regardless of how stiff or soft the specimen becomes.

F controlled loading is different. Number of oil injections necessary to keep F "on target" vary with specimen stiffness. If a system was near linear elastic, there would be no problem, but stiffness can change a lot in sand specimens, thus F-PID control can fail. PID controller calibrated "too stiff" can resonate – oscillate out of control (see Fig.3). Whereas relaxed values cause F-PID to lag behind the F target. This makes applying F cycles on liquefying specimens very complicated. Standard PID controllers are simply not robust enough.

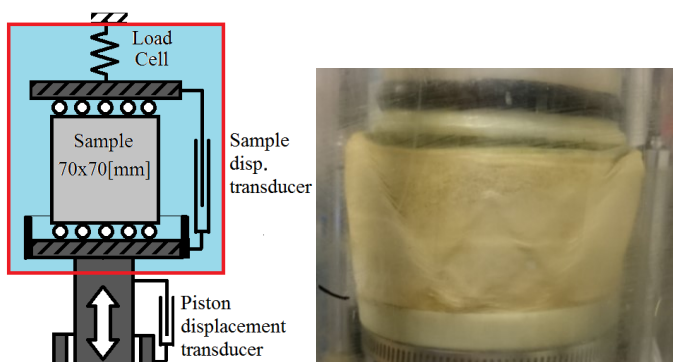


Fig. 1 Schematic of test setup and axially compressed (20% strain) dry, unsaturated Aalborg no.1 sand, resulting in 6 overlapping shear bands.

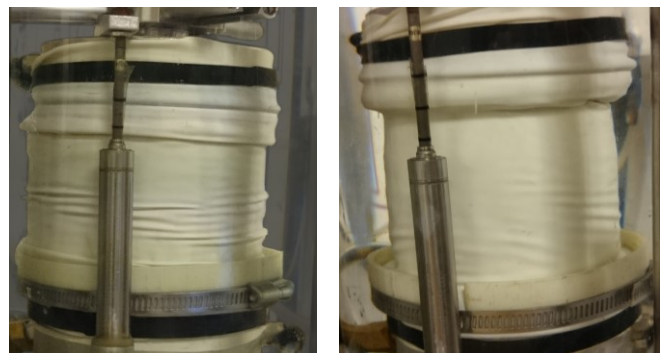


Fig. 2 Saturated, undrained samples. 10% axial compression strain on the left. On the right - 6 times compressed to failure, pulled to initial length and drained with cyclic testing in between. Geometry remained satisfactory.

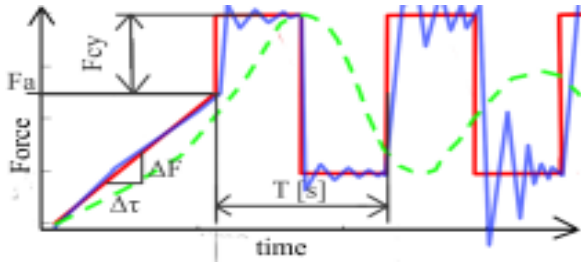


Fig. 4 Square wave loading with 2 cases of bad tuning illustrated on top

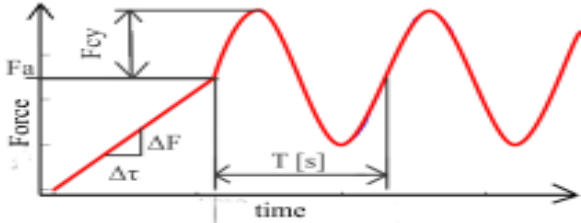


Fig. 5 Sinusoidal loading shape.

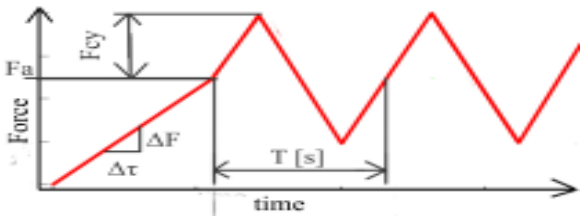


Fig. 6 Saw tooth loading

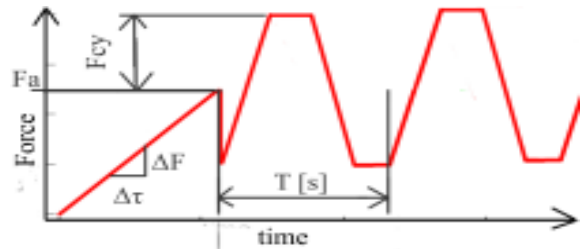


Fig. 3 Trapezoid loading

### Square wave loading

Square wave (Fig.3) has very steep transition from one peak to another. This makes it great for tuning the PID controller, as square waves expose resonance or overdamping. PID control has 3 coefficients – position, integral and derivative. These three determine how aggressively the piston reaches for the target. The three are normally calibrated through trial and error, while the test is running.

In F mode, PID coefficients depend on specimen stiffness. The number of oil injections required to reach target F changes with specimen stiffness. Thus, different parameters of F-PID are necessary at different stiffness. However, no such problems are present during U-PID calibration: hydraulic piston is grossly overpowered, thus the correlation between U and oil injections remains the same, regardless of the specimen stiffness. Which makes U-PID calibration stable at all times.

### Sinusoidal loading

Sinusoid wave (Fig.4) has smooth curves, making it easier for F-PID to catch up with real time measurements at the peaks. This wave shape is stable over a wider range of specimen stiffness, as the smooth shape reduces the danger of resonating and/or under/over-loading a specimen. But during liquefaction it was found impossible to maintain a stable sinusoidal shape using F-PID control (shown in Fig.7).

### Saw tooth loading

Cycles of linear ramp unloading/reloading can be combined into a saw-tooth pattern (Fig. 6). This is advantageous for testing deformation cycles. The loading rate ( $du$ ) is constant during such loading cycles, this allows to isolate individual components within equation of motion:

$$F=K \cdot u+C \cdot du+M \cdot ddu \quad (1)$$

Where  $u$  is displacement,  $du = \Delta U/\Delta t$  (first derivative, loading rate),  $ddu$  – second derivative (acceleration). And  $K$ ,  $C$  and  $M$  are stiffness, damping and mass components. To model dynamic sand response, the  $K$ ,  $C$  and  $M$  need to be treated as nonlinear functions. Therefore it is crucial to isolate them one at a time. If  $U$  cycles are applied at increasingly slower  $du$ , a quasi-static  $K$  will emerge. Once  $K$  curvature is quasi-static, further reduction in  $du$  will not produce changes in measurement. But if  $du$  is increased (cycle frequency increased), the quasi-static stiffness path will start changing, and the deviation will be caused by  $C$  component. Thus, U-PID saw-tooth loads allow to separate  $K$  from  $C$ , from  $M$ , all behaving like nonlinear state dependants.

### Trapezoid loading

If saw-tooth peaks are paused for a brief moment – trapezoidal wave is shaped (Fig.6). The flat peaks can be used for observing stress relaxation (U-PID) and strain creep (F-PID) with each cycle. Allowing specimens to stabilize at the peaks can ensure quasi-static response is being measured.

### STRAIN AND STRESS VS U AND F

The default control methods are limited to F and U control. Yet, specimens are tested for stress and strain. Thus, it would be good if U and F could be applied in ways which target stress and strain. This is where standard PID is modified to meet triaxial testing.

Converting piston U to specimen strain takes some compromises. Piston displacement does not match specimen deformation "exactly". As Fig.1 shows, piston displacement is re-distributed between the specimen and the load cell (load cell deforms like a spring too). However, the load cell is a very stiff spring. Even more so during liquefaction, when the specimen becomes soft, and in a series spring system, the softest spring absorbs largest proportion of deformation (in this case, the specimen absorbs most of the deformation). Thus, even though PID control has no access to real specimen deformation, the

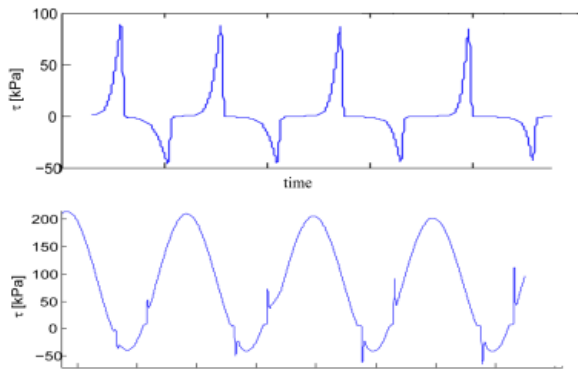


Fig. 7 Performance of script loading (top) compared with F PID controlled sinusoidal loading (bottom), acting on liquefying specimen.

piston position can be used as a close substitute. Especially during liquefaction.

Given these observations, true strain can be obtained as:

$$\varepsilon = \ln \left( 1 - \frac{\Delta U}{H_0} \right) \quad (2)$$

Where  $H_0$  is initial specimen height. In addition, undrained specimens have constant volume – thus, predictable cross-section to obtain stresses from. True (absolute) stress can be obtained as:

$$\tau = \frac{q}{2} = (F/A_0) \cdot (1 + \varepsilon) \quad (3)$$

Where  $A_0$  is the initial cross-section area of a specimen, and  $(1 + \varepsilon)$  accounts for change in cross-section during loading. Note, here the stress measured is "absolute", not "effective".

Absolute (undrained) stress limits are predictable. Firstly, undrained yielding always occurs when pore pressure drops to near -100 kPa, thus undrained yielding can be predicted by monitoring real time pore pressure. Secondly, undrained yielding strength can be approximated with equation:

$$\tau_{min,max} = \frac{(C_p + 100) \cdot \tan \varphi}{\frac{2}{3} \cdot \tan \varphi \pm 1} \quad (4)$$

where  $C_p$  and  $\varphi$  are the chamber pressure and the friction angle, respectively. The constant of 100 kPa, representing cavitation limit. The theoretical limit for cavitation is 100kPa (absolute vacuum), but in tests, cavitation of de-aired specimens occurred near -85 kPa. Thus, using 85 (or slightly less) instead of 100 could be an option providing more realistic estimates.

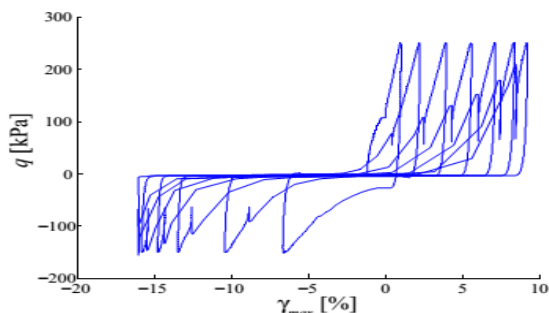


Fig. 8 Force controlled liquefaction response (REF SOREN). If loaded further the first of "double peaks" will go beyond the maximum stress level.

## LIQUEFACTION

The challenge of measuring liquefaction in cyclic loaded specimens, using the Danish triaxial apparatus was attempted by Nielsen & Ibsen, 2013. Two way loaded sinusoidal F-PID cycles were applied, and the PID controlled produced "overshooting" peaks (visible in bottom picture of Fig.7).

Overshoot occurs because of rapidly changing stiffness of liquefied specimens. There is a "pure plastic gap" when crossing  $q=0$  axis, thus changes in stiffness are tremendous when loading direction is reversed (see Fig.9). In pure plastic zone F-PID will produce acceleration which will accumulate into large loading velocity (du component). F-PID accelerates and de-accelerates with a minor delay, thus, it will not be able to stop once the target F is reached. And to make matters worse, after F-PID exceeds the target F it will attempt to unload assuming linear stiffness. But unloading stiffness is much steeper in sand, thus the "overshoot" will be followed by "undershoot". This F-PID behavior cannot be prevented using the PID coefficients. Make the piston more aggressive and it will oscillate out of control around the target F value. Relax the settings – and overloading/under-loading will get worse. However, U-PID has no such problems. U-PID is unconditionally stable. The only problem is targeting F values using U-PID for input.

### Targeting F using U-PID

The problem with using U-PID is that F plays no role in U-PID algorithm. One has to specify the targeted U and the U-PID will control oil injections required to reach the U target. Thus, to target F instead, it is necessary to monitor real time F values, and change the targeted U value once the F limits are reached. Luckily, the MOOG station allows to monitor real time F using scripts (Troya & Sabaliauskas, 2014). Furthermore, not only F limits can be observed, but F can be converted into  $\tau$  within the script using Eq's (2,3).

A script can take measurement of F a few thousand times per second. Measurements can be converted to  $\tau$  within the same millisecond, and du direction is reversed once  $\tau$  peak is reached. The principle is very simple, each time  $\tau$  peak is triggered, loading direction is reversed (see Fig. 9). However, it

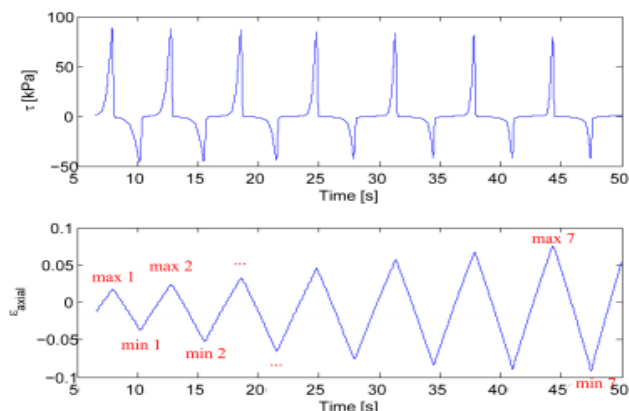


Fig. 9 Adopting strain controlled liquefaction loading. Stress time series on top. Strain time series in the bottom.



is not enough to merely reverse displacement direction, the loading period needs to be preserved. The distance between peak U positions is increasing with each loading cycles, thus the  $du$  value has to be updated after every peak – to cover the next distance faster (or slower) depending on how the peak position evolves during the test.

Notice how  $\epsilon$  distance is smaller between  $max1-min1$  compared to  $max7-min7$  in Fig.9. The "gap" between the peaks is increasing as specimens liquefy. This is easy to account for if  $du$  component (loading rate) is updated after each peak crossing. Distance between  $min1$  to  $min2$  needs to be crossed with:  $du=(max1-min1)/T$ , and distance between  $max7$  to  $min 7$  is crossed with  $du=(max7-min6)/T$ . This allows to update  $du$  with respect to previous loading cycle. This does not provide the exact solution, as loading rate is slightly too slow, but in Fig.9 one can see the period is rather stable, and close to  $T=11$ .

### Limitations

It must be noted, that F-PID is problematic only at high plasticity, and during periods of unstable stiffness. Otherwise, when stiffness is near linear, F-PID performs really well. At times when stiffness is very steep, F-PID is the only real option. At high stiffness, U-PID scripts becomes unstable, as small deformation creates large F fluctuations. Therefore, care must be taken to select the correct setting:

1. U-PID for testing nonlinear, pure plastic behavior
2. F-PID for testing linear, elastic behavior.

### FUTURE WORK

Using U-PID loading, specimens survive through aggressive liquefaction. Thus, post liquefaction soil states can be researched. This is interesting for researching soil states left after earthquakes. As well as disturbed soil states encountered by offshore wind turbines.

The new testing scope allows to iterate between liquefaction and draining, which allows reach very high densities, which could not be accessed using alternative preparation methods. The specimens can be densified to the point of purely dilative state. Such "exotic" soil state (pure dilative) could be very interesting to research as a fundamental boundary limit of sand.

Foundations of structures built offshore must function in cyclic loaded environment. Thus, liquefaction and drained post-liquefaction recovery are both important. The control algorithms developed thus far are sufficient to safely liquefy, drain and re-liquefy specimens. Thus, evolution full complexity of disturbed sand stiffness can be observed.

### Introducing new capabilities

Besides new testing capabilities already available, the equipment is not perfect. Some modifications can be implemented to improve it further. At the moment, two computers are connected to the (dynamic) Danish triaxial apparatus. One of them is dedicated to data acquisition. The second one – PID controller. The two computers do not communicate with each other. The PID controlled has no access

to data describing the specimen itself. If the two computers were upgraded to share a common database, a whole new level of automation would become plausible: Scripts could be written to target specific densities of a specimen. Specimens could be "reset" to initial stiffness, to make data tables autonomously. Pore pressure measurements would allow to prevent undrained specimens from yielding more efficiently. In the most farfetched scenario machine learning algorithms could be implemented for data mining. Sand has extremely nonlinear stiffness, complexity of which quickly overwhelms a human observer. Given how durable and stable the specimens are, it could be plausible to generate state space maps and decision trees (such as Markov decision process) by allowing a machine learning algorithm to explore the patterns autonomously.

### CONCLUSION

The new found capability to test liquefied sand is stable and reliable. A specimen can be liquefied, and continued to test thereafter. As specimen durability is improved, it becomes plausible to increase complexity and aggressiveness of testing, which in turn provide access to new observations – new knowledge.

Some remaining limitations of the equipment cannot be surpassed without partial reconstruction of equipment – such as combining the separate computers into one unit. But it seems new testing scope can be reached by merely changing the software, rather than upgrading the hardware. The testing capabilities of frictionless triaxial apparatus are not exhausted yet, the equipment can reach observations far beyond conventional testing limits.

### BIBLIOGRAPHY

- Hettler, A. & Vardoulakis, I., 1984. *Behaviour of dry sand tested in a large triaxial apparatus*. s.l.:Geotechnique 34.2 (1984): 183-197..
- Nielsen, S. D. & Ibsen, L. B., 2013. s.l.:International Society of Offshore and Polar Engineers.
- Praastrup, U., Jakobsen, K. P. & Ibsen, L. B., 1999. *Two Theoretically Consistent Methods for Analysing Triaxial Tests*. Aalborg: Computers and Geotechnics. Vol. 25(1999), pp. 157-170.
- Sabaliauskas, T. & Troya, A., 2014. *Observations during static and cyclic undrained loading of dense Aalborg University sand no. 1*. Aalborg: DCE Technical Memorandum No. 43.
- Shajarati, A., Sørensen, K. W., Dam, S. K. & Ibsen, L. B., 2012. *Manual for Cyclic Triaxial Test*. Aalborg: DCE Technical Report No. 114.
- Troya, A. & Sabaliauskas, T., 2014. *Cyclic behaviour of undrained dense Aalborg University sand no. 1*. Aalborg: DCE Technical Memorandum. Department of Civil Engineering, Aalborg University,.
- Ibsen, L. B., 1995. *The Static and Dynamic Strength of Sand*. Copenhagen: European Conference on Soil Mechanics and Foundation Engineering.

## **Recent publications in the DCE Technical Report Series**

The making of Andersen's liquefaction chart  
Sabaliauskas, T. & Ibsen, L. B.  
2017, DCE Technical Memorandum; No. 62.

