



Aalborg Universitet

AALBORG UNIVERSITY  
DENMARK

## Is Regression Gain or Instantaneous Gain the most reliable and reproducible gain value when performing video Head Impulse Testing of the lateral semicircular canals?

Jacobsen, Chris Ladefoged; Abrahamsen, Emil Riis; Skals, Regitze Kuhr; Hougaard, Dan Dupont

*Publication date:*  
2018

*Document Version*  
Publisher's PDF, also known as Version of record

[Link to publication from Aalborg University](#)

*Citation for published version (APA):*  
Jacobsen, C. L., Abrahamsen, E. R., Skals, R. K., & Hougaard, D. D. (2018). *Is Regression Gain or Instantaneous Gain the most reliable and reproducible gain value when performing video Head Impulse Testing of the lateral semicircular canals?*. Poster presented at 31st Politzer Society Meeting & 2nd Global Otology Research Forum, Las Palmas de Grand Canaria, Spain.

### General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal -

### Take down policy

If you believe that this document breaches copyright please contact us at [vbn@aub.aau.dk](mailto:vbn@aub.aau.dk) providing details, and we will remove access to the work immediately and investigate your claim.

# Is Regression Gain or Instantaneous Gain the most reliable and reproducible gain value when performing video Head Impulse Testing of the lateral semicircular canals?

Chris L. Jacobsen<sup>1</sup>, Emil R. Abrahamsen<sup>1,3</sup>, Regitze K. Skals<sup>2</sup>, Dan D. Hougaard<sup>1,3</sup>

<sup>1</sup>Department of Otolaryngology, Head & Neck Surgery and Audiology, Aalborg University Hospital, Aalborg, Denmark, <sup>2</sup>Unit of Clinical Biostatistics and Bioinformatics, Aalborg University Hospital, Aalborg, Denmark, <sup>3</sup>Department of Clinical Medicine, Aalborg University Hospital, Aalborg, Denmark

## Introduction

With the advancement of vestibular testing modalities, the video Head Impulse Test (v-HIT) has earned a prominent place in the clinical setting. It is now possible to test all of the semi-circular canals (SCCs) fast and efficiently.

The v-HIT systems provide information about the function of the vestibular ocular reflex (VOR) by means of two modalities: SACCADES and GAIN (the ratio between eye and head velocities).

The EyeSeeCam® v-HIT system presents the gain value as:

- **Regression gain** (a best fitted line through the data plots)
- **Instantaneous gain** value at 40, 60 and 80ms. (The mean value at specific latencies)

## Objective

### Primary endpoint:

- Is instantaneous gain or regression gain the most reproducible and reliable gain value when performing v-HIT with testing of the lateral SCCs?

### Secondary endpoints :

- Comparison of each of the instantaneous gain values at 40, 60, and 80ms with the regression gain values of the lateral SCCs.
- Investigate any intra- and inter examiner variability when comparing gain values between an inexperienced and an experienced neurotologist.

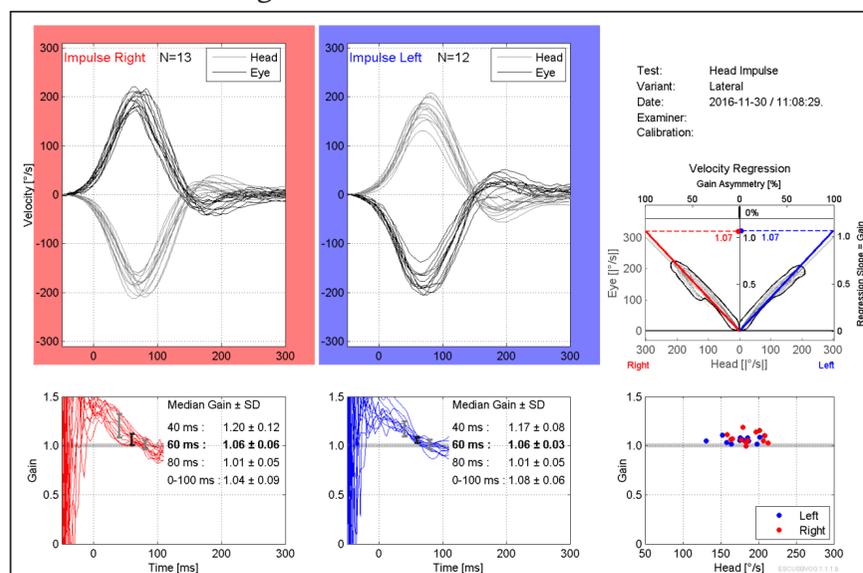


Fig. 1 Report after lateral SCC testing of a person without vestibular pathology depicting both Instantaneous and Regression gain.

## Materials

The v-HIT system -EyeSeeCam® from Interacoustics, Denmark, was used to perform the v-HIT tests on all lateral SCCs.

## Methods

60 subjects between 18-65 years without any prior history of vestibular disease were included.

Prior to inclusion all subjects filled out a questionnaire as well as the Dizziness Handicap Inventory (DHI). All subjects underwent testing with video frenzel goggles to rule out nystagmus and eye muscle disorders.

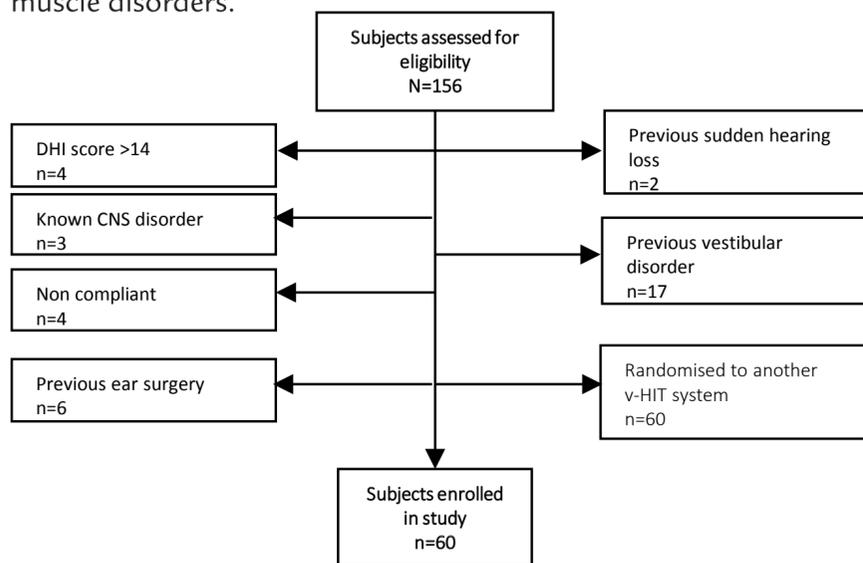


Fig. 2 Trial profile

All subjects underwent two complete v-HIT test sessions by an experienced and an inexperienced examiner respectively. The order of the examiners and the sequence of the SCC being tested were randomized.

## Results

- When testing the lateral SCCs we found that the regression gain was the most reproducible gain value when comparing it with instantaneous gain.

Instantaneous Gain vs. Regression Gain	mean sd	95% ci	p-value
Regression Gain	0.05	[0.03;0.06]	<0.001
Instantaneous gain vs. regression gain	0.02	[0.01;0.03]	<0.001
Right lateral vs. Left lateral	0.02	[0.00;0.02]	0,005

Table 1 Instantaneous vs regression gain with regression gain as reference

- When comparing the individual instantaneous gain values (40, 60, 80ms) with the regression gain, we found that the gain values at 40ms had the greatest standard deviation (sd) when comparing with regression gain (p-value <0.001, 95% ci [0.03;0.05] mean sd 0.04)
- When holding instantaneous gain latencies up against each other there was significant deviation at 40ms but not at 60 nor 80ms.

Instantaneous gain 60ms as reference	mean sd	95% ci	p-value
Instantaneous gain 40ms	0.033	[0.02;0.04]	<0.001
Instantaneous gain 80ms	0.001	[-0.01;0.01]	0,809

Table 2 Instantaneous gain values at 40 and 80ms compared to 60ms

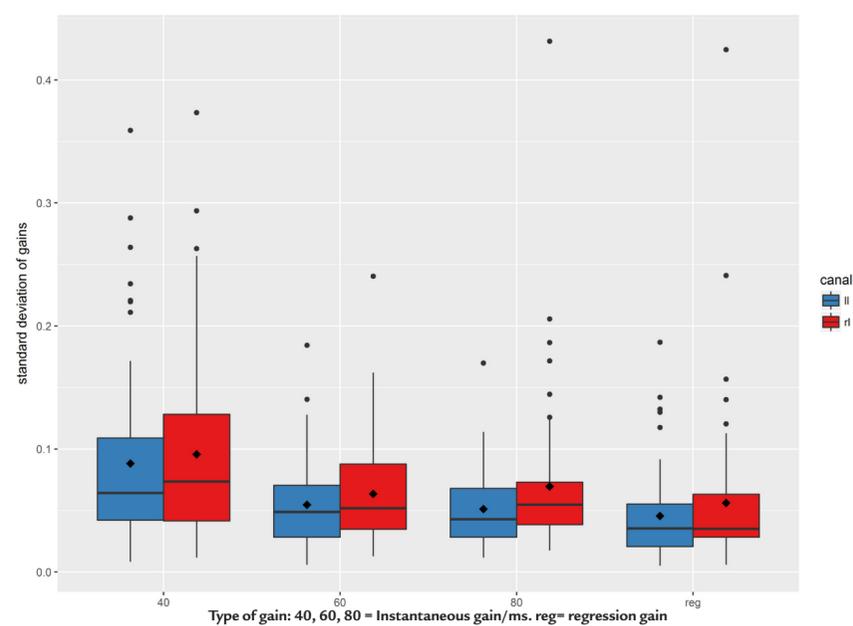


Fig. 3 Mean standard deviation of the different gain types.

- When comparing the experienced to the inexperienced doctor no significant gain deviation was found.

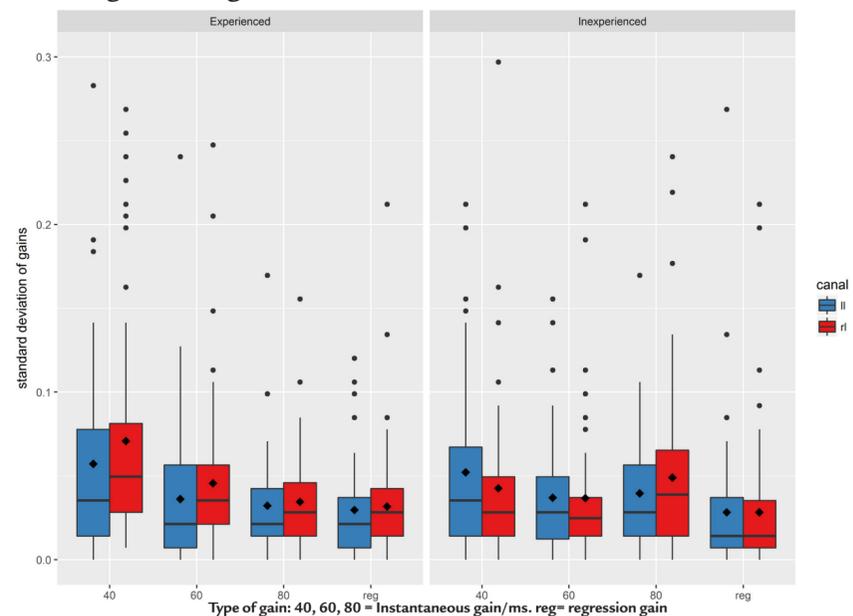


Fig. 4 Standard deviations of the different gain types performed by the experienced/inexperienced doctor.

## Conclusion

- Regression gain is more reproducible than instantaneous gain.
- 40ms is the least reproducible of the instantaneous values.
- There was no significant difference at 60ms or 80ms of the instantaneous gain.
- No significant intra or inter examiner variability (experienced/inexperienced)

## References

- Halmagyi, G. M., Chen, L., MacDougall, H. G., Weber, K. P., McGarvie, L. A., & Curthoys, I. S. (2017). The video head impulse test. *Front Neurol*. <https://doi.org/10.3389/fneur.2017.00258>
- Korsager, L. E. H., Schmidt, J. H., Faber, C., & Wanscher, J. H. (2016). Reliability and comparison of gain values with occurrence of saccades in the EyeSeeCam video head impulse test (vHIT). *Eur Arch Otorhinolaryngol*, 273(12), 4273–4279. <https://doi.org/10.1007/s00405-016-4183-2>
- Abrahamsen, ER, Christensen, AE, and Hougaard, DD (2018) Intra- and Interexaminer Variability of Two Separate Video Head Impulse Test Systems Assessing All Six Semicircular Canals. *Otol Neurotol* (volume 39 issue 2 pages e113-e122)
- Janky KL, Patterson JN, Sheppard NT, Thomas MLA, Honaker JA (2017) Effects of Device on Video Head Impulse Test (vHIT) Gain. *J Am Acad Audiol Oct*;28(9):778-785. doi: 10.3766/jaaa.16138.
- Cleworth TW, Carpenter MG, Honegger F, Allum JHJ. (2017) Differences in head impulse test results due to analysis techniques. *J Vestib Res*. 2017;27(2-3):163-172. doi: 10.3233/VES-170614.
- EyeSeeCam manual, Interacoustic, Rev 3 -ver.11/2013.